

**Model PM4-IV**  
**Panel Mount Display/Controller**  
**Operation and Instruction Manual**

---

*AMALGAMATED INSTRUMENT CO PTY LTD*

*ACN: 001 589 439*

*Unit 5, 28 Leighton Place Hornsby  
NSW 2077 Australia*

*Telephone: +61 2 9476 2244  
Facsimile: +61 2 9476 2902*

*e-mail: sales@aicpl.com.au  
Internet: www.aicpl.com.au*

# Table of Contents

<b>1</b>	<b>Introduction</b>	<b>3</b>
<b>2</b>	<b>Mechanical Installation</b>	<b>4</b>
<b>3</b>	<b>Electrical installation</b>	<b>5</b>
<b>4</b>	<b>Function tables - summary of setup functions</b>	<b>11</b>
<b>5</b>	<b>Explanation of functions</b>	<b>16</b>
<b>6</b>	<b>Calibration</b>	<b>42</b>
<b>7</b>	<b>Setting up the relay PI controller</b>	<b>46</b>
<b>8</b>	<b>Specifications</b>	<b>56</b>
<b>9</b>	<b>Guarantee and service</b>	<b>57</b>

# 1 Introduction

## 1.1 General description

This manual contains information for the installation and operation of the PM4-IV Panel Mount Monitor. The PM4-IV is a general purpose instrument which may be configured to accept an input signal of  $\pm 2\text{mA}$ ,  $\pm 20\text{mA}$ , 4 to 20mA,  $\pm 100\text{mV}$ ,  $\pm 1\text{V}$ ,  $\pm 10\text{V}$ ,  $\pm 100\text{VDC}$  or 3 wire slidewire ( $0\text{-}1\text{k}\Omega$  to  $0\text{-}1\text{M}\Omega$ ). The PM4-IV offers the choice of linear or square root display. Two separate sets of calibration scaling values can be stored with the display choice being made via the remote input (e.g. voltage free switch). The instrument may be scaled by the user to display the input in engineering units e.g. mm, RPM, Litres etc.. The PM4-IV is available in 4, 5, 6 or 5 digit plus bargraph LED display form or with 4 or 6 digit LCD display.

The PM4 series of Panel Mount Monitors are designed for high reliability in industrial applications. The high brightness LED display provides good visibility even in areas with high ambient light levels. The high contrast LCD displays provide good visibility and are ideal for battery powered applications. Full electrical isolation between power supply, input voltage or current and retransmission output is provided by the PM4, thereby eliminating grounding and common voltage problems. This isolation feature makes the PM4 ideal for interfacing to computers, PLCs and other data acquisition devices. Unless otherwise specified at the time of order, your PM4 has been factory set to a standard configuration. The PM4 series instruments can be configuration and calibrated easily by the user. Initial changes may require dismantling the instrument to alter PCB links, other changes are made by push button functions.

## 1.2 Standard outputs

- A standard inbuilt relay provides an alarm/control function (can be set for on/off alarm/control or PI control using pulse width or frequency control)
- A non isolated transmitter supply of approx. 18VDC (25mA max.) regulated is provided.


## 1.3 Output options

- 1, 3 or 6 extra relays (first optional relay can be set for simple on/off alarm/control or PI control using pulse width or frequency control)
- Isolated analog retransmission (single or dual analog outputs) configurable for 4–20mA., 0–1V or 0–10V. The first analog output is configurable for retransmission or PI control
- $\pm 12\text{VDC}$  (24V) isolated transmitter supply/excitation voltage (25mA max.). Not to be used with the standard 18VDC transmitter supply
- Isolated RS485 or RS232 serial communications (ASCII or Modbus RTU)
- Isolated Digital output - binary or BCD up to 16 bit, NPN or PNP output types available
- Isolated Optional outputs are available in certain combinations e.g. Extra relay plus RS232

## 2 Mechanical Installation

Choose a mounting position as far away as possible from sources of electrical noise such as motors, generators, fluorescent lights, high voltage cables/bus bars etc. An IP65 access cover which may be installed on the panel and surrounds is available as an option to be used when mounting the instrument in damp/dusty positions. A wall mount case is available, as an option, for situations in which panel mounting is either not available or not appropriate. A portable carry case is also available, as an option, for panel mount instruments.

Prepare a panel cut out of 45mm x 92mm +1 mm / - 0 mm (see diagram below). Insert the instrument into the cut out from the front of the panel. From the rear of the instrument fit the two mounting brackets into the recess provided (see diagram below). Whilst holding the bracket in place, tighten the securing screws being careful not to over-tighten, as this may damage the instrument. Hint: use the elastic band provided to hold the mounting bracket in place whilst tightening securing screws.

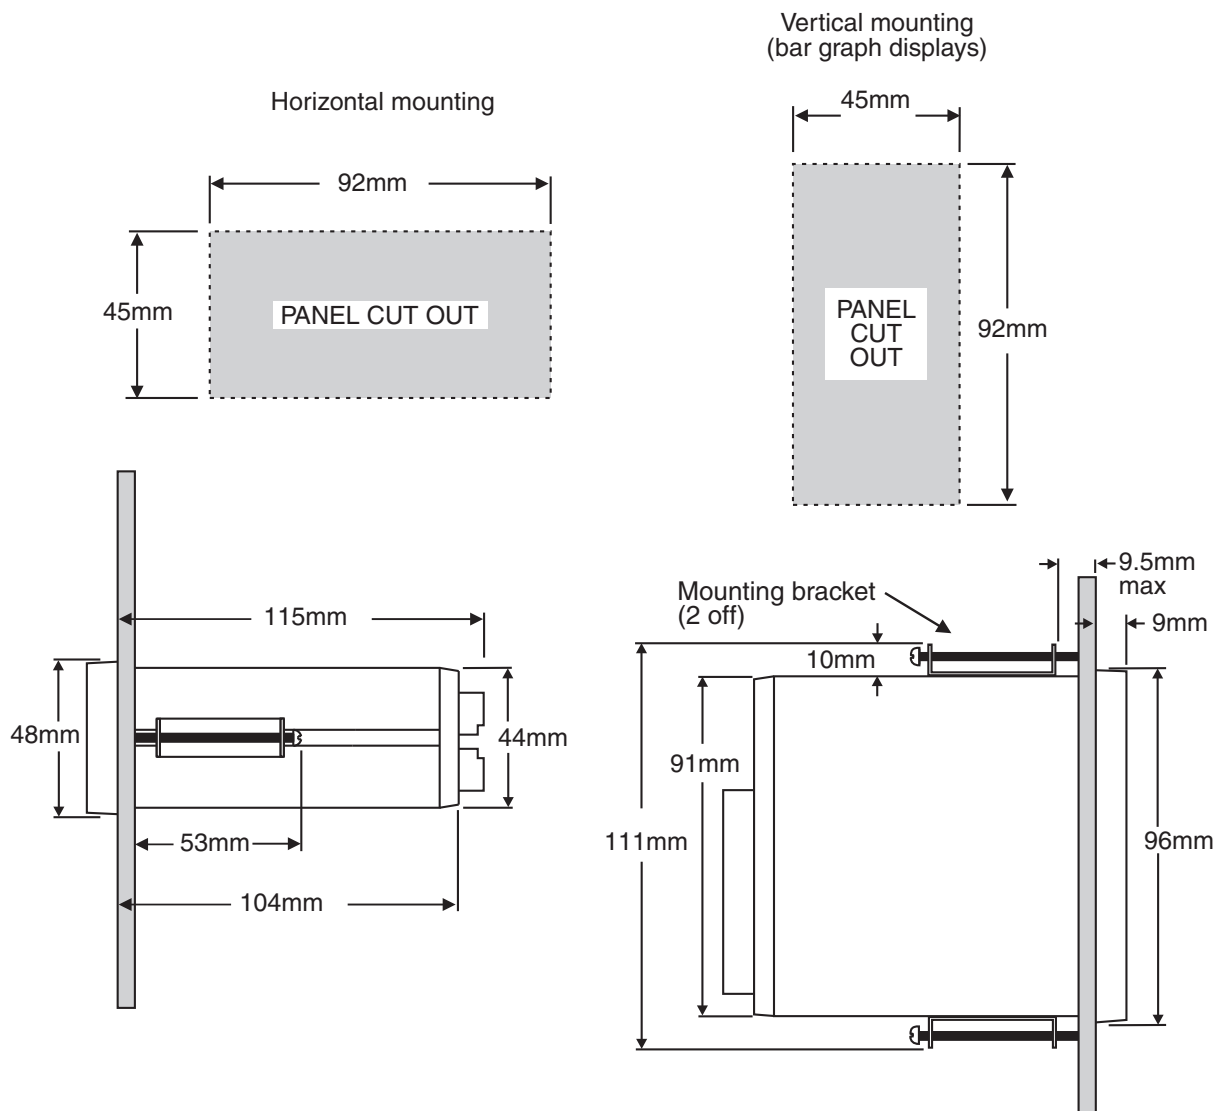

# 3 Electrical installation


## 3.1 Electrical installation

The PM4 Panel Meter is designed for continuous operation and no power switch is fitted to the unit. It is recommended that an external switch and fuse be provided to allow the unit to be removed for servicing.

The plug in, screw type, terminal blocks allow for wires of up to 2.5mm<sup>2</sup> to be fitted. Connect the wires to the appropriate terminals as indicated below. Refer to connection details provided in this chapter to confirm proper selection of voltage, polarity and input type before applying power to the instrument.

When power is applied the instrument will cycle through a display sequence indicating the software version and other status information, this indicates that the instrument is functioning. Acknowledgement of correct operation may be obtained by applying an appropriate input to the instrument and observing the reading. The use of screened cable is recommended for signal inputs.

For connection details of optional outputs refer to the separate "PM4 Panel Meter Optional Output Addendum" booklet supplied when options are fitted.

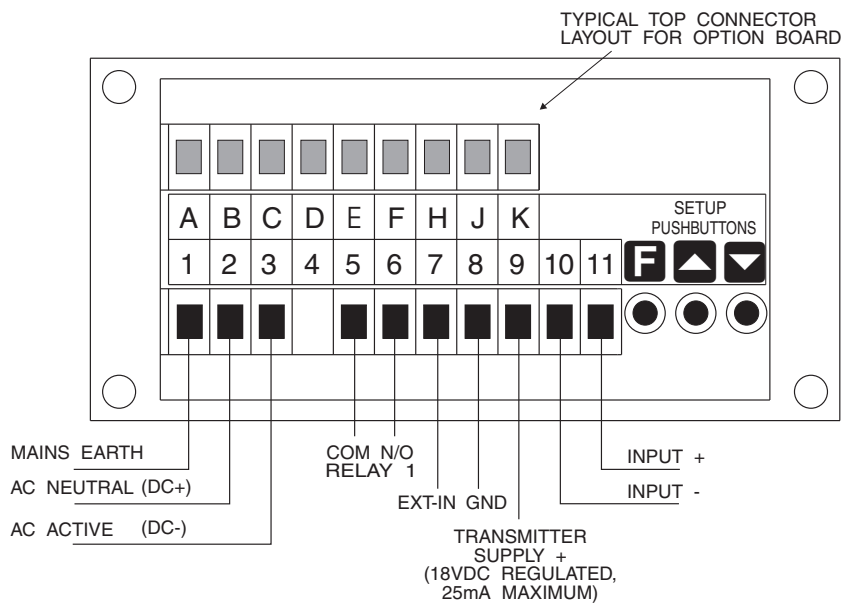


1	MAINS EARTH	
2	240VAC NEUTRAL	
3	240VAC ACTIVE	
5	RELAY 1	COM
6	RELAY 1	N/O
7	EXT IN	
8	GND	
9	SUPPLY	+18VDC
10	INPUT	-VE
11	INPUT	+VE
PM4-IV-240-5E		SERIAL No.

Instrument data label (example)


### 3.2 Electrical connection examples

If output options are fitted refer to the "PM4 Panel Meter Optional Output Addendum" booklet for connection details.


AC power connections - supply type is factory configured, check before connecting

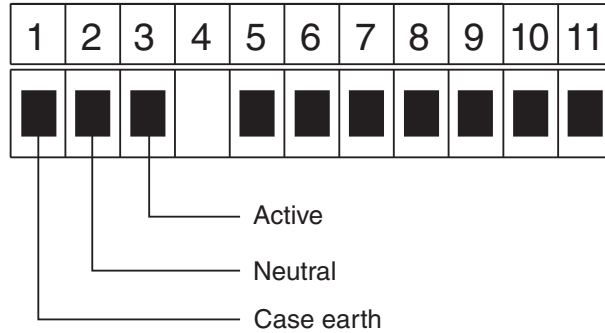


DC power connections (12 to 48VDC) - supply type is factory configured, check before connecting

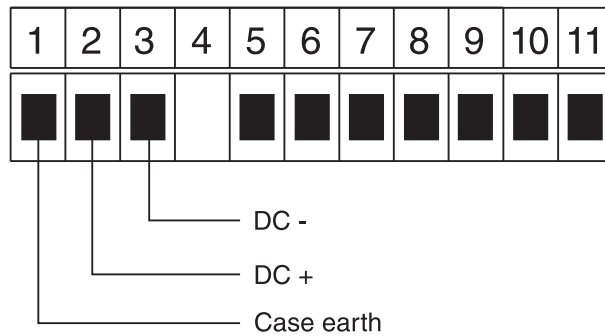


2 wire 4-20mA powered from non isolated regulated 18V supply (25mA maximum)

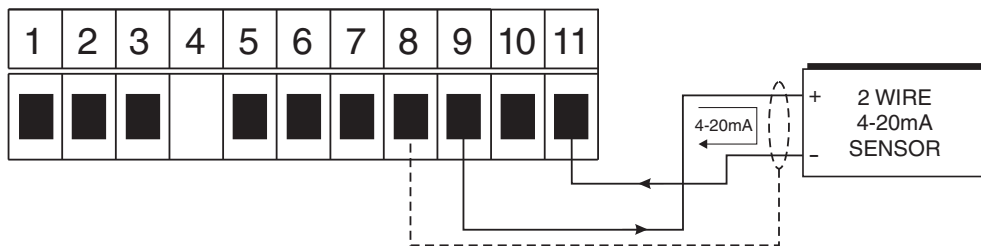


2 wire 4-20mA externally powered sensor

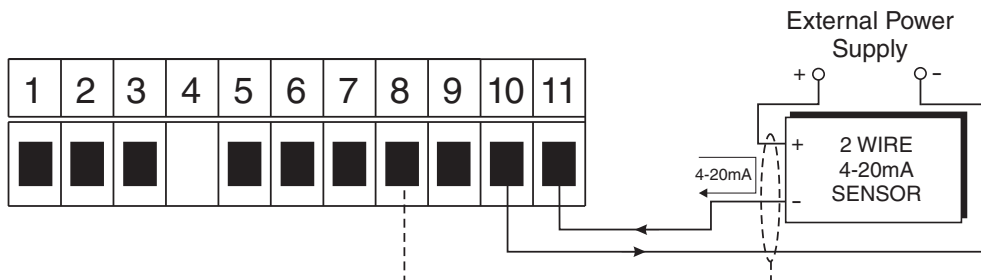


3 wire 4-20mA externally powered sensor

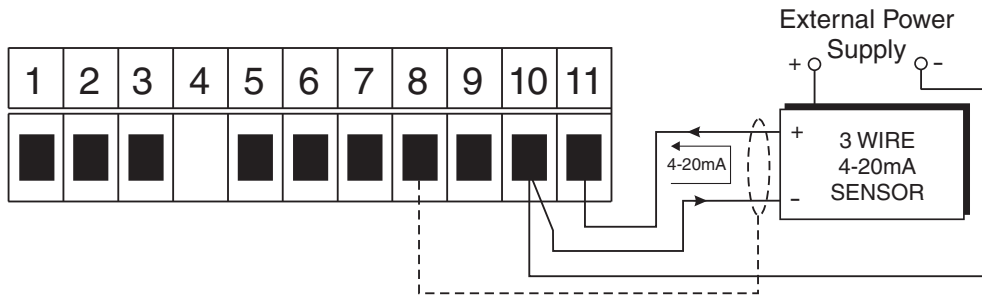


4 wire 4-20mA externally powered sensor

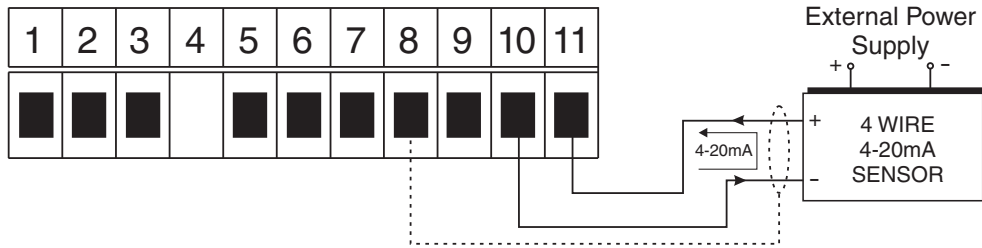


3 wire 4-20mA powered from non isolated regulated 18V supply (25mA maximum)

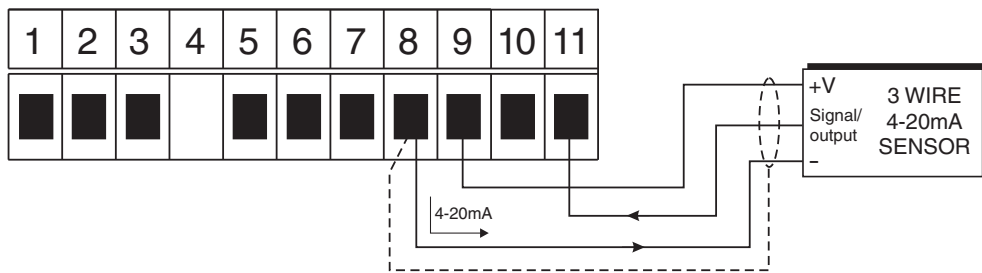


2 wire 4-20mA powered from optional isolated regulated 24V (± 12V) supply (25mA maximum)

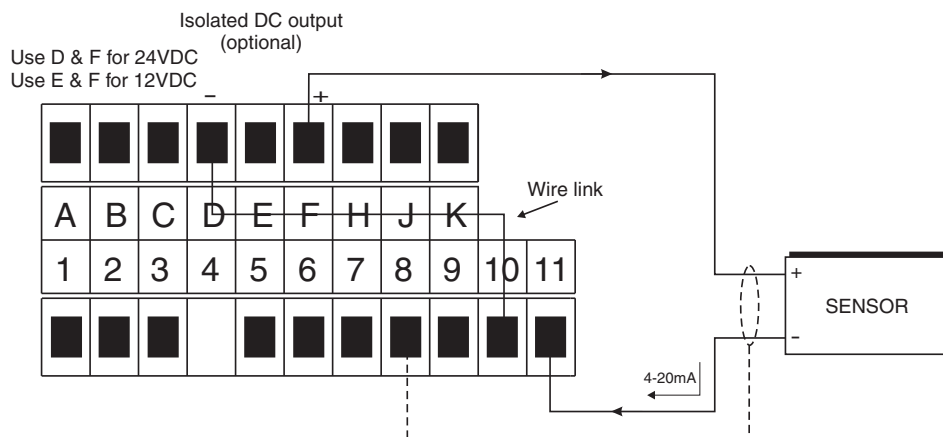


DC voltage input

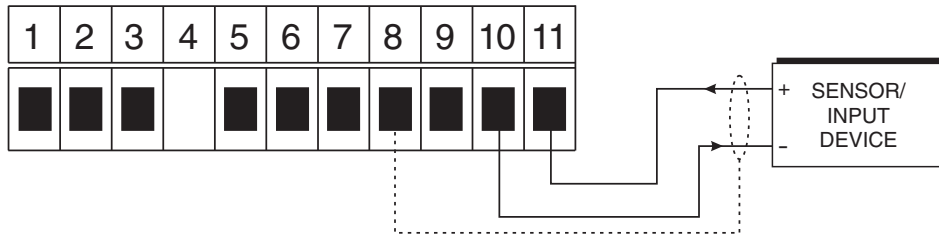

Slidewire input

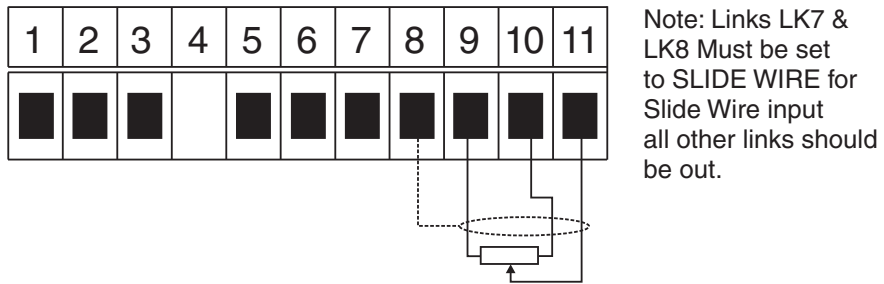


Remote input

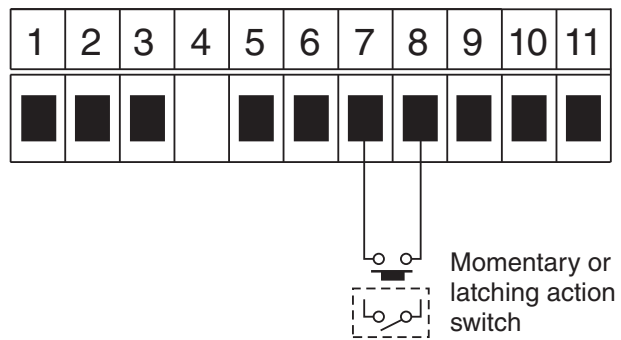


### 3.3 Input Output Configuration

If you need to alter the input or output configuration link settings proceed as follows:


1. Remove the plug in terminals from the rear of the instrument

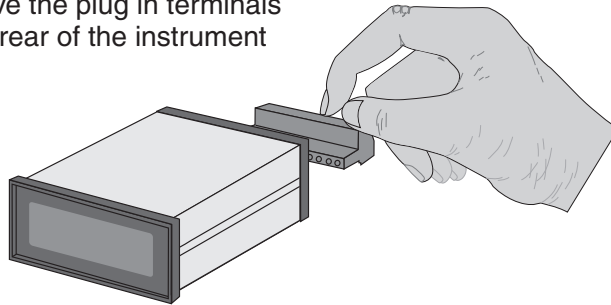

2. Remove the 4 x self tapping screws from the back cover then remove the back cover by pulling it away from the instrument

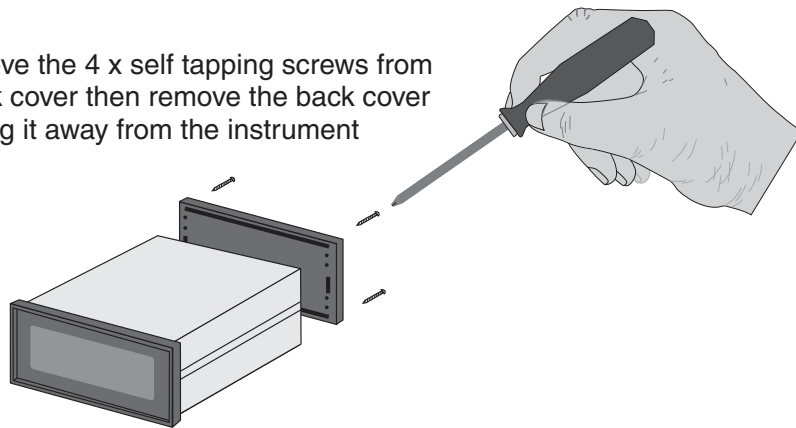

3. Remove the earth screw which passes through the underside of the case then slide out the board or boards

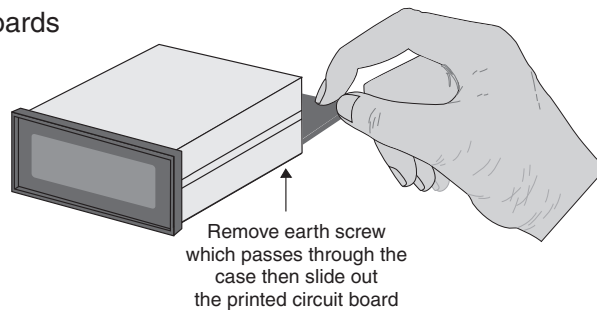

4. Configure the PCB links as required, see appropriate chapter
5. Slide PCB back into case
6. Replace the earth screw which passes through the case
7. Refit the back cover and fix with the self tapping screws
8. Plug the terminal strips back into the rear of the instrument



## 4 Function tables - summary of setup functions

Note: the order in which the functions appear on the display may not be exactly as shown below. The availability and order of functions is determined by choice of function settings and options fitted.

Functions in this first table are available in **FUNC** or **CAL** mode

Display	Function	Range	Default	Your record	Ref/Page
<b>RxLo</b>	Low setpoint value for designated alarm relay <i>x</i>	Any display value or <b>OFF</b>	<b>OFF</b>	See 4.1	5.1 / 18
<b>RxHi</b>	High setpoint value for designated alarm relay <i>x</i>	Any display value or <b>OFF</b>	<b>OFF</b>	See 4.1	5.2 / 18
<b>RxHy</b>	Hysteresis value for the designated alarm relay <i>x</i> .	<b>0</b> to <b>9999</b>	<b>10</b>	See 4.1	5.3 / 19
<b>Rxtt</b>	Trip time delay for the designated alarm relay <i>x</i> .	<b>0</b> to <b>9999</b>	<b>0</b>	See 4.1	5.4 / 20
<b>Rxrt</b>	Reset time delay for the designated alarm relay <i>x</i> .	<b>0</b> to <b>9999</b>	<b>0</b>	See 4.1	5.5 / 20
<b>Rxn.o</b> or <b>Rxn.c</b>	Alarm relay <i>x</i> action to normally open (de-energised) or normally closed (energised)	<b>Rxn.o</b> or <b>Rxn.c</b>	<b>Rxn.o</b>	See 4.1	5.6 / 20
<b>RxSP</b> or <b>Rxt i</b> etc.	Relay operation independent setpoint or trailing setpoint (*Optional)	<b>RxSP</b> or <b>Rxt i</b> etc.	<b>RxSP</b>	See 4.1	5.7 / 21
<b>Rx.SP</b>	PI relay control setpoint	Any display value	<b>0</b>	See 4.1	7.2 / 47
<b>brgt</b>	Display brightness level	<b>1</b> to <b>15</b>	<b>15</b>		5.9 / 22
<b>dull</b>	Display remote brightness switching	<b>0</b> to <b>15</b>	<b>1</b>		5.10 / 22
<b>P.SET</b>	Preset value	Any display value	<b>0</b>		5.11 / 22

(\*Optional)—this function will only be accessible if the relevant option is fitted

Functions in this second table are available only in **CAL** mode or if **ACCS** is set to **ALL**

Display	Function	Range	Default	Your record	Ref/Page
<b>Rx OPEr</b>	Relay operation mode, alarm or PI control	<b>Rx.AL</b> or <b>Rx.tP</b> or <b>Rx.Fr</b>	<b>Rx.AL</b>	See 4.1	5.8 / 21
<b>ctrl SPAN</b>	PI relay control span	Any display value	<b>100</b>	See 4.1	7.3 / 47
<b>Rx.P9</b>	PI relay proportional gain	<b>-32.767</b> to <b>32.767</b>	<b>0.0 10</b>	See 4.1	7.4 / 48
<b>Rx.I 9</b>	PI relay integral gain	<b>-32.767</b> to <b>32.767</b>	<b>0.000</b>	See 4.1	7.5 / 49
<b>Rx.I L</b>	PI relay integral control low limit	<b>0.0</b> to <b>100.0</b>	<b>100.0</b>	See 4.1	7.6 / 50
<b>Rx.I H</b>	PI relay integral control high limit	<b>0.0</b> to <b>100.0</b>	<b>100.0</b>	See 4.1	7.7 / 51
<b>Rx.bs</b>	PI relay control output bias	<b>0.0</b> to <b>100.0</b>	<b>50.0</b>	See 4.1	7.8 / 51
<b>Rx.dc</b>	PI relay control cycle period	<b>0</b> to <b>250</b>	<b>10</b>	See 4.1	7.9 / 52
<b>Rx.dr</b>	PI relay on duration	<b>0.0</b> to <b>25.0</b>	<b>1.0</b>	See 4.1	7.12 / 54
<b>bAr -</b>	Bargraph low value (*Optional)	Any display value	<b>0</b>		5.12 / 23
<b>bAr ~</b>	Bargraph high value (*Optional)	Any display value	<b>1000</b>		5.13 / 23
<b>bAr tYPE</b>	Bargraph type (*Optional)	<b>bAr</b> , <b>S.dot</b> , <b>d.dot</b> <b>C.bAr</b> or <b>r.dot</b>	<b>bAr</b>		5.14 / 23
<b>d9OP</b>	Digital output option mode (*Optional)	<b>bcd</b> , <b>b.SCL</b> , <b>b, n</b> or <b>b, n2</b>	<b>b, n2</b>		5.15 / 24
<b>d9.OP</b>	Digital output option polarity (*Optional)	<b>AI o</b> or <b>AI,</b>	<b>AI o</b>		5.16 / 24
<b>bcd Start</b>	Digital output option BCD start position (*Optional)	Any display value	<b>0</b>		5.17 / 25
<b>d, 9 -</b>	Digital output option low value (*Optional)	Any display value	<b>0</b>		5.18 / 25
<b>d, 9 ~</b>	Digital output option high value (*Optional)	Any display value	<b>1000</b>		5.19 / 25
<b>FECC -</b>	Analog output option low display value (*Optional)	Any display value	<b>0</b>		5.20 / 26

(\*Optional)—this function will only be accessible if the relevant option is fitted

<b>FEC<sup>-</sup></b>	Analog output option high display value ( <b>*Optional</b> )	Any display value	<b>1000</b>		5.21 / 26
<b>FEC<sub>-CH2</sub></b>	Second analog output option low display value ( <b>*Optional</b> )	Any display value	<b>0</b>		5.22 / 26
<b>FEC<sup>-</sup><sub>CH2</sub></b>	Second analog output option high display value ( <b>*Optional</b> )	Any display value	<b>1000</b>		5.23 / 27
<b>drnd</b>	Display rounding	<b>1 to 5000</b>	<b>1</b>		5.24 / 27
<b>dCPt</b>	Decimal point	<b>0, 0.1</b> etc.	<b>0</b>		5.25 / 27
<b>FLtr</b>	Digital filter	<b>0 to 8</b>	<b>2</b>		5.26 / 27
<b>di SP unit</b>	Display unit	<b>NONE, °C, °F, °C, or F</b>	<b>NONE</b>		5.27 / 28
<b>CAL 1</b>	First live input calibration scaling point	Any display value	<b>0</b>		5.28 / 28
<b>CAL 2</b>	Second live input calibration scaling point	Any display value	<b>1000</b>		5.29 / 28
<b>CAL OFFst</b>	Calibration offset	Any display value	n/a		5.30 / 29
<b>ZERO RANGE</b>	Zero range limit	Any display value or <b>OFF</b>	<b>OFF</b>		5.31 / 29
<b>CAL ZERO</b>	Zero point calibration	n/a	n/a		5.32 / 29
<b>USEF En4</b>	4mA input scale	Any display value	n/a		5.33 / 29
<b>USEF En20</b>	20mA input scale	Any display value	n/a		5.34 / 29
<b>UCAL</b>	Uncalibrate	n/a	n/a		5.35 / 30
<b>rEcctri</b>	Analog output PI control ( <b>*Optional</b> )	<b>on</b> or <b>OFF</b>	<b>OFF</b>		5.36 / 30
<b>Pbut</b>	<b>P</b> button function (for instruments with front <b>P</b> button)	<b>NONE, Hi, Lo, Hi, Lo, tARF, ZERO, P.SET or O.Put</b>	<b>NONE</b>		5.37 / 30
<b>FINP</b>	Remote input (external input) one function	<b>NONE, P.HLd, d.HLd, Hi, Lo, Hi, Lo, tARF, ZERO, SP.Ac, No.Ac, CAL.S, P.SET, duLL or O.Put</b>	<b>NONE</b>		5.38 / 31

(\*Optional)—this function will only be accessible if the relevant option is fitted

<b>NETT FLSH</b>	Nett flash inhibit	<b>on</b> or <b>OFF</b>	<b>OFF</b>		5.39 / 33
<b>ACCS</b>	Access mode	<b>OFF.EASY.</b> <b>NONE</b> or <b>ALL</b>	<b>OFF</b>		5.40 / 34
<b>SPAC</b>	Setpoint access mode (*Optional)	<b>A1.A1-2</b> etc.	<b>A1</b>		5.41 / 34
<b>SQRt</b>	Square root mode	<b>on</b> or <b>OFF</b>	<b>OFF</b>		5.42 / 34
<b>A1.A2</b> etc.	Alarm relay operation mode	<b>L, UE, tARFE.</b> <b>P.HLd.</b> <b>d.HLd.H, .</b> <b>Lo</b> or <b>di SP</b>	<b>L, UE</b>	See 4.1	5.43 / 35
<b>bARF</b>	Bargraph display operation mode (*Optional)	<b>L, UE, tARFE.</b> <b>P.HLd.</b> <b>d.HLd.H, .</b> <b>Lo</b> or <b>di SP</b>	<b>L, UE</b>		5.44 / 36
<b>rEC</b> or <b>rEE2</b> or <b>d9.OP</b> or <b>SEFL</b>	Analog /digital/serial operation mode (*Optional)	<b>L, UE, tARFE.</b> <b>P.HLd.</b> <b>d.HLd.H, .</b> <b>Lo</b> or <b>di SP</b>	<b>L, UE</b>		5.45 / 37
<b>Lo</b> <b>di SP</b>	Low overrange visual warning limit value	Any display value or <b>OFF</b>	<b>OFF</b>		5.46 / 38
<b>Hi GH</b> <b>di SP</b>	High overrange visual warning limit value	Any display value or <b>OFF</b>	<b>OFF</b>		5.47 / 38
<b>di SP</b>	Display visual warning flashing mode	<b>FLSH</b> or <b>-or-</b>	<b>FLSH</b>		5.48 / 38
<b>bAUD</b>	Baud rate for serial communications (*Optional)	<b>300.600.</b> <b>1200.2400.</b> <b>4800.9600.</b> <b>19.2</b> or <b>38.4</b>	<b>9600</b>		5.49 / 39
<b>Prty</b>	Parity for serial communications (*Optional)	<b>NONE.EVEN</b> or <b>odd</b>	<b>NONE</b>		5.50 / 39
<b>Q.Pwt</b>	Output for serial communications (*Optional)	<b>di SP.Cont.</b> <b>POLL, A.buS</b> or <b>ā.buS</b>	<b>Cont</b>		5.51 / 39
<b>Addr</b>	Instrument address for serial communications (*Optional)	<b>0</b> to <b>31</b>	<b>0</b>		5.52 / 39
<b>SEFL</b>	Serial mode for serial communications (*Optional)	<b>L, UE, tARFE.</b> <b>P.HLd.</b> <b>d.HLd.H, .</b> <b>Lo.H, Lo</b> or <b>di SP</b>	<b>L, UE</b>		5.53 / 40

(\*Optional)—this function will only be accessible if the relevant option is fitted

## 4.1 Relay table

Record your relay settings in the table below

Display	Relay 1	Relay 2	Relay 3	Relay 4	Relay 5	Relay 6	Relay 7
<b>RxLo</b>							
<b>RxHi</b>							
<b>RxHY</b>							
<b>Rxtt</b>							
<b>Rxrt</b>							
<b>Rxn.o</b> or <b>Rxn.c</b>							
<b>RxSP</b> or <b>Rxt I</b> etc.	n/a						
<b>R1,R2</b> etc.							
<b>RxOPER</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.SP</b>			n/a	n/a	n/a	n/a	n/a
<b>ctrl SPAN</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.P9</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.I9</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.I L</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.I H</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.bs</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.dc</b>			n/a	n/a	n/a	n/a	n/a
<b>Rx.dr</b>			n/a	n/a	n/a	n/a	n/a

## 5 Explanation of functions

The PM4 setup and calibration functions are configured through a push button sequence. The three push buttons located at the rear of the instrument (also at the front on some display options) are used to alter settings. Two basic access modes are available:

**FUNC** mode (simple push button sequence) allows access to commonly set up functions such as alarm setpoints.

**CAL** mode (power up sequence plus push button sequence) allows access to all functions including calibration parameters.

Once **CAL** or **FUNC** mode has been entered you can step through the functions, by pressing and releasing the **F** push button, until the required function is reached. Changes to functions are made by pressing the or push button (in some cases both simultaneously) when the required function is reached. See the flow chart example on the following page.


### Entering **CAL** Mode



1. Remove power from the instrument. Hold in the **F** button and reapply power. The display will briefly indicate **CAL** as part of the "wake up messages" when the **CAL** message is seen you can release the button. Move to step 2 below.



2. When the "wake up" messages have finished and the display has settled down to its normal reading press, then release the **F** button. Move to step 3 below.



3. Within 2 seconds of releasing the **F** button press, then release the **▲** and **▼** buttons together. The display will now indicate **FUNC** followed by the first function.


Note: If step 1 above has been completed then the instrument will remain in this **CAL** mode state until power is removed. i.e. there is no need to repeat step 1 when accessing function unless power has been removed.

### Entering **FUNC** Mode

No special power up procedure is required to enter **FUNC** mode.




1. When the "wake up" messages have finished and the display has settled down to its normal reading press, then release the **F** button.




2. Within 2 seconds of releasing the **F** button press, then release the **▲** and **▼** buttons together. The display will now indicate **FUNC** followed by the first function.

Example: Entering **FUNC** mode to change alarm 1 high function **ALH**, from **OFF** to **100**

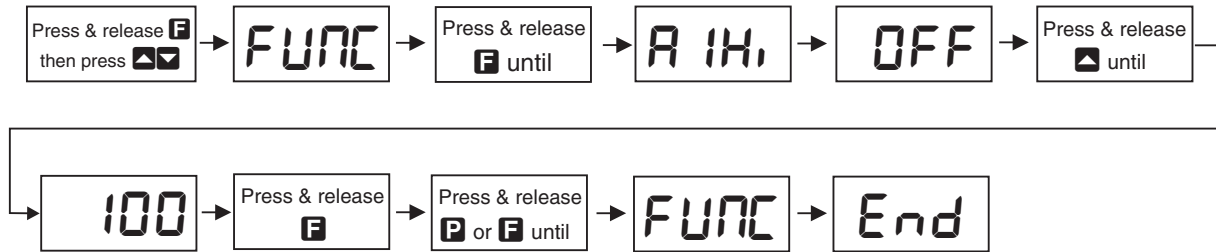

Example: Entering **CAL** mode to change decimal point function **dCPT** from **0** to **0.02**

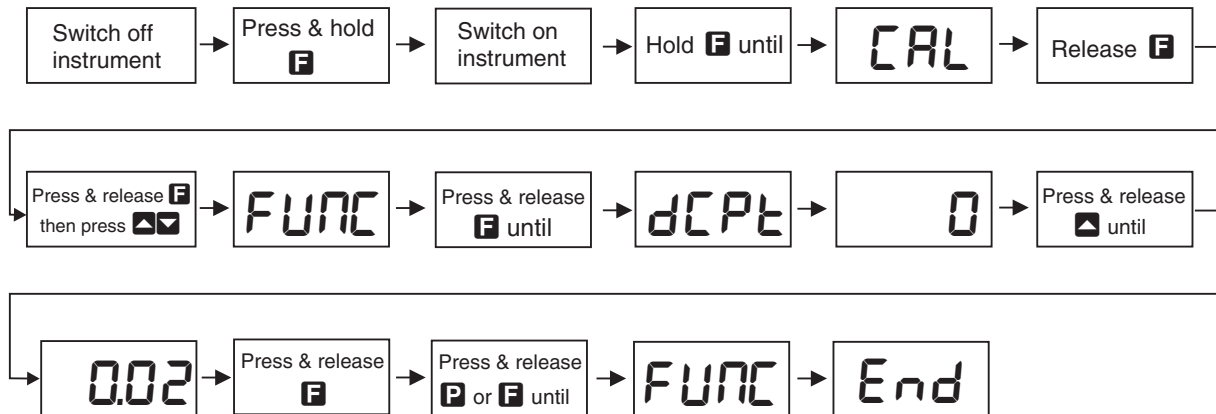

### Easy alarm relay adjustment access facility

The display has an easy alarm access facility which allows access to the alarm setpoints simply by pressing the **F** button at the front or rear of the instrument. The first setpoint will then appear and changes to this setpoint may be made to this setpoint via the **▲** or **▼** buttons. Press the **F** button to accept any changes or to move on to the next setpoint. Note: this easy access also functions in the same manner for the PI control setpoint (relay and/or analog PI output) if PI control is available. The instrument must be set in the manner described below to allow the easy access facility to work:

1. The **F: NP** function must be set to **SPAC** or the **ACCS** function must be set to **EASY**.
2. At least one alarm must have a setpoint, nothing will happen if all the alarm setpoints are set to **OFF**.
3. The **SPAC** function must be set to allow access to the relays required e.g. if set to **A 1-2** then the easy access will work only with alarm relays 1 and 2 even if more relays are fitted.
4. The instrument must be in normal measure mode i.e. if the instrument is powered up so that it is in **CAL** mode then the easy access will not function. If in doubt remove power from the instrument, wait for a few seconds then apply power again.
5. If the easy access facility is used then the only way to view or alter any other function settings is to power up via **CAL** mode i.e. there is no entry to **FUNC** mode functions unless the instrument is powered up in **CAL** mode.

# Explanation of Functions


## 5.1 Alarm relay low setpoint

**Display:**  $RxLo$   
**Range:** Any display value or **OFF**  
**Default Value:** **OFF**

Displays and sets the low setpoint value for the designated alarm relay  $x$ . Note  $x$  will be replaced by the relay number when displayed e.g.  $R1Lo$  for relay 1. Use this low setpoint function if a relay operation is required when the display value becomes equal to or less than the low setpoint value. To set a low alarm value go to the  $RxLo$  function and use the  $\blacktriangle$  or  $\blacktriangledown$  push buttons to set the value required then press **F** to accept this value. The low alarm setpoint may be disabled by pressing the  $\blacktriangle$  and  $\blacktriangledown$  push buttons simultaneously. When the alarm is disabled the display will indicate **OFF**. If the relay is allocated both a low and high setpoint then the relay will activate when the value displayed moves outside the band set by the low and high setpoints. The value at which the relay will reset is controlled by the  $RxHy$  function.

### Example:

If  $R1Lo$  is set to **10** then relay 1 will activate when the display value is 10 or less.

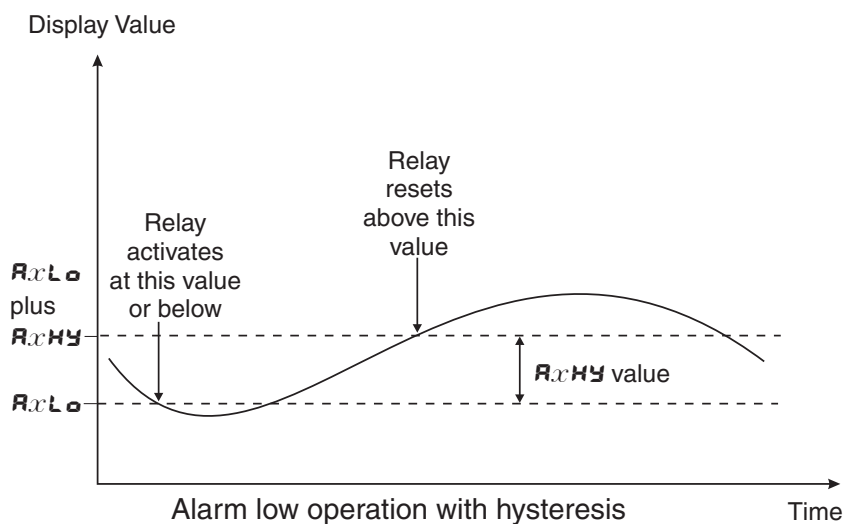

## 5.2 Alarm relay high setpoint


**Display:**  $RxH$   
**Range:** Any display value or **OFF**  
**Default Value:** **OFF**

Displays and sets the high setpoint value for the designated alarm relay  $x$ . Note  $x$  will be replaced by the relay number when displayed e.g.  $R1H$  for relay 1. Use this high setpoint function if a relay operation is required when the display value becomes equal to or more than the low setpoint value. To set a high alarm value go to the  $RxH$  function and use the  $\blacktriangle$  or  $\blacktriangledown$  push buttons to set the value required then press **F** to accept this value. The high alarm setpoint may be disabled by pressing the  $\blacktriangle$  and  $\blacktriangledown$  push buttons simultaneously. When the alarm is disabled the display

will indicate **OFF**. If the relay is allocated both a low and high setpoint then the relay will activate when the value displayed moves outside the band set by the low and high setpoints. The value at which the relay will reset is controlled by the **RxHY** function.

**Example:**

If **R1H** is set to **100** then relay 1 will activate when the display value is **100** or higher.

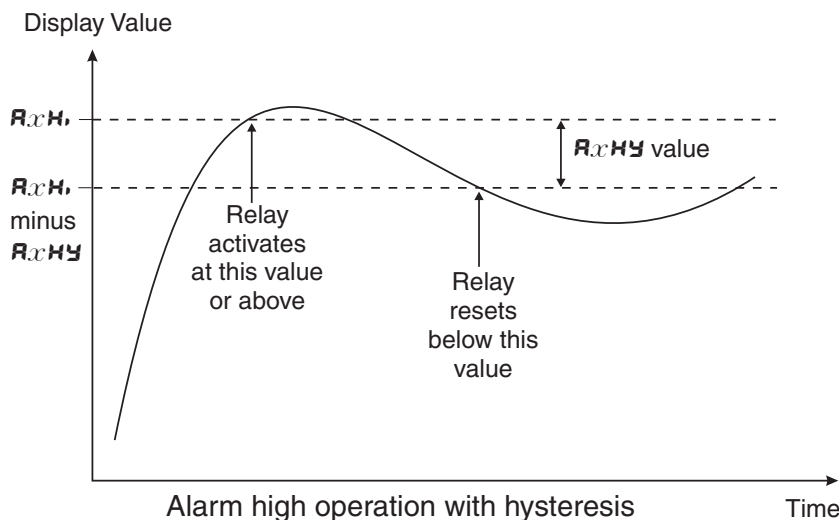

### 5.3 Alarm relay hysteresis (deadband)

Display: **RxHY**  
 Range: **0 to 9999**  
 Default Value: **10**

Displays and sets the alarm relay hysteresis limit for the designated relay *x*. Note *x* will be replaced by the relay number when displayed e.g. **R1HY** for relay 1. To set a relay hysteresis value go to the **RxHY** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value. The hysteresis value is common to both high and low setpoint values. The hysteresis value may be used to prevent too frequent operation of the relay when the measured value is rising and falling around setpoint value. e.g. if **R1HY** is set to zero the alarm will activate when the display value reaches the alarm setpoint (for high alarm) and will reset when the display value falls below the setpoint, this can result in repeated on/off switching of the relay at around the setpoint value. The hysteresis setting operates as follows: In the high alarm mode, once the alarm is activated the input must fall below the setpoint value minus the hysteresis value to reset the alarm. e.g. if **R1H** is to **50.0** and **R1HY** is set to **3.0** then the setpoint output relay will activate once the display value goes to **50.0** or above and will reset when the display value goes below **47.0** i.e. at **46.9** or below. In the low alarm mode, once the alarm is activated the input must rise above the setpoint value plus the hysteresis value to reset the alarm. e.g. if **R1L** is to **20.0** and **R1HY** is set to **10.0** then the alarm output relay will activate when the display value falls to **20.0** or below and will reset when the display value goes above **30.0** i.e at **30.1** or above. The hysteresis units are expressed in displayed engineering units.

**Example:**

If **R1H** is set to **100** and **R1HY** is set to **10** then relay 1 will activate when the display value is **100** or higher and will reset at a display value of **89** or lower.

## 5.4 Alarm relay trip time

**Display:** **Ax<sub>t</sub>t**  
**Range:** **0** to **9999**  
**Default Value:** **0**

Displays and sets the alarm trip time in seconds. The trip time is common for both alarm high and low setpoint values. The trip time provides a time delay before the alarm relay will activate when an alarm condition is present. The alarm condition must be present continuously for the whole trip time period before the alarm will activate. If the input moves out of alarm condition during this period the timer will reset and the full time delay will be restored. This trip time delay is useful for preventing an alarm trip due to short non critical deviations from setpoint. The trip time is selectable over **0** to **9999** seconds. To set a trip time value go to the **Ax<sub>t</sub>t** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value.

### Example:

If **A<sub>1</sub>t** is set to **5** seconds then the display must indicate an alarm value for a full 5 seconds before relay 1 will activate.

## 5.5 Alarm relay reset time

**Display:** **Ax<sub>r</sub>t**  
**Range:** **0** to **9999**  
**Default Value:** **0**

Displays and sets the alarm reset delay time in seconds. The reset time is common for both alarm high and low setpoint values. With the alarm condition is removed the alarm relay will stay in its alarm condition for the time selected as the reset time. If the input moves back into alarm condition during this period the timer will reset and the full time delay will be restored. The reset time is selectable over **0** to **9999** seconds. To set a reset time value go to the **Ax<sub>r</sub>t** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value.

### Example:

If **A<sub>1</sub>r** is set to **10** seconds then the resetting of alarm relay 1 will be delayed by 10 seconds.

## 5.6 Alarm relay normally open/closed

**Display:** **Ax<sub>n.o</sub>** or **Ax<sub>n.c</sub>**  
**Range:** **Ax<sub>n.o</sub>** or **Ax<sub>n.c</sub>**  
**Default Value:** **Ax<sub>n.o</sub>**

Displays and sets the setpoint alarm relay *x* action to normally open (de-energised) or normally closed (energised), when no alarm condition is present. Since the relay will always open when power is removed a normally closed alarm is often used to provide a power failure alarm indication. To set the alarm alarm for normally open or closed go to the **Ax<sub>n.o</sub>** or **Ax<sub>n.c</sub>** function and use the **▲** or **▼** push buttons to set the required operation then press **F** to accept this selection.

### Example:

If set to **A In.o** alarm relay 1 will be open circuit when the display is outside alarm condition and will be closed (short circuit across terminals) when the display is in alarm condition.

## 5.7 Alarm relay setpoint or trailing operation

**Display:** **AxSP** or **Ax.t 1** etc.

**Range:** **AxSP** or **Ax.t 1** etc.

**Default Value:** **AxSP**

Relay operation independent setpoint or trailing setpoint, this function will not be seen unless extra optional relays are fitted. Each alarm, except relay 1, may be programmed to operate with an independent setpoint value or may be linked to operate at a fixed difference to another relay setpoint, known as trailing operation. The operation is as follows:

Alarm 1 (**A1**) is always independent. Alarm 2 (**A2**) may be independent or may be linked to Alarm 1. Alarm 3 (**A3**) may be independent or may be linked to Alarm 1 or Alarm 2. Alarm 4 (**A4**) may be independent or may be linked to Alarm 1, Alarm 2 or Alarm 3. The operation of each alarm is selectable by selecting, for example, (Alarm 4) **A4.SP** = Alarm 4 normal setpoint or **A4.t 1** = Alarm 4 trailing Alarm 1 or **A4.t 2** = Alarm 4 trailing Alarm 2 or **A4.t 3** = Alarm 4 trailing Alarm 3. For trailing set points the setpoint value is entered as the difference from the setpoint being trailed. If the trailing setpoint is to operate ahead of the prime setpoint then the value is entered as a positive number and if operating behind the prime setpoint then the value is entered as a negative number.

### Example:




With Alarm 2 set to trail alarm 1, if **A1H** is set to **1000** and **A2H** is set to **50** then Alarm 1 will activate at **1000** and alarm 2 will activate at **1050** (i.e. 1000 + 50). If Alarm 2 had been set at **-50** then alarm 2 would activate at **950** (i.e. 1000 - 50).

## 5.8 Alarm relay operation mode

**Display:** **Ax OPER**

**Range:** **Ax.AL** or **Ax.tP** or **Ax.Fr**

**Default Value:** **Ax.AL**

Alarm relay operating mode (relays 1 and 2 only) - this function allows selection of standard alarm on/off setpoint operation (**A1.AL** or **A2.AL**) using the alarm functions described in this chapter or PI control operation (**A1.tP** or **A1.Fr** or **A2.tP** or **A2.Fr**). To set the alarm operation mode go to the **Ax OPER** function and use the  or  push buttons to choose the required operation then press  to accept this value.

Refer to the “Setting up the relay PI controller” chapter 7 for details of the PI control operations and functions.

### Example:

With **Ax OPER** set to **A1.Fr** relay 1 will operate as a PI control relay with the frequency of the relay varying.

## 5.9 Display brightness

**Display:** **br9t**  
**Range:** **1** to **15**  
**Default Value:** **15**

Displays and sets the digital display brightness. The display brightness is selectable from **1** to **15**, where **1** = lowest intensity and **15** = highest intensity. This function is useful for improving the display readability in dark areas or to reduce the power consumption of the instrument. See also the **dull** function 5.10. To set brightness level go to the **br9t** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value.

## 5.10 Display remote brightness switching

**Display:** **dull**  
**Range:** **0** to **15**  
**Default Value:** **1**

Displays and sets the level for remote input brightness switching, see **r.inp** function. When a remote input is set to **dull** the remote input can be used to switch between the display brightness level set by the **br9t** function 5.9 and the display brightness set by the **dull** function. The display dull level is selectable from **0** to **15**, where **0** = lowest intensity and **15** = highest intensity. This function is useful in reducing glare when the display needs to be viewed in both light and dark ambient light levels. To set dull level go to the **dull** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value.

### Example:

With **dull** set to **4** and **br9t** set to **15** and the **r.inp** function set to **dull** the display brightness will change from the **15** level to **4** when a switch connected to the remote input terminals is activated.

## 5.11 Preset value

**Display:** **P.SET**  
**Range:** Any display value  
**Default Value:** **0**




A preset value can be entered at this function. If a remote input (**r.inp** function) or **P** button (function) is programmed to **P.SET** then operation of the remote input or **P** button will cause the display to change to the preset value. Any change in input from this point will cause a variation above or below the preset value. To set preset value go to the **P.SET** function and use the **▲** or **▼** push buttons to set the value required then press **F** to accept this value.

### Example:

With a display showing a value of **50** at a given input if the **P.SET** function is set to **70** and the remote function is set to **P.SET** then once the remote input is activated the same input will now have a display value of **70**.




## 5.12 Bargraph low value

**Display:** `bAr_`  
**Range:** Any display value  
**Default Value:** `0`

Seen only in bargraph display instruments. Displays and sets the bar graph low value i.e. the value on the 7 segment display at which the bargraph will start to rise. This may be independently set anywhere within the display range of the instrument. Note: The `bAr_` and `bAr^` settings are referenced from the 7 segment display readings, not the bargraph scale values. The bargraph scale may scaled differently to the 7 segment display. For example the bargraph scale may be indicating percentage fill of a tank whilst the 7 segment display is indicating actual process units. To set bargraph low level go to the `bAr_` function and use the  or  push buttons to set the value required then press  to accept this value.

## 5.13 Bargraph high value

**Display:** `bAr^`  
**Range:** Any display value  
**Default Value:** `1000`

Seen only in bargraph display instruments. Displays and sets the bar graph high value i.e. the value on the 7 segment display at which the bargraph will reach its maximum indication (e.g. all LEDs illuminated). May be independently set anywhere within the display range of the instrument. To set bargraph high level go to the `bAr^` function and use the  or  push buttons to set the value required then press  to accept this value.

## 5.14 Bargraph type

**Display:** `bAr tYPE`  
**Range:** `bAr`, `S.dot`, `d.dot` `C.bAr` or `r.dot`  
**Default Value:** `bAr`

Bar graph display operation mode - seen only in vertical or circular bargraph display instruments. Allows selection of bargraph operation mode. Choices available are:

- `bAr` - conventional solid bargraph display i.e. all LEDs illuminated when at full scale. When scaling the display use the `bAr_` and `bAr^` functions e.g. `bAr_ = 0` and `bAr^ = 100` will give a bargraph with no segments lit at a 7 segment display reading of `0` and all segments lit with a 7 segment display reading of `100`.
- `S.dot` - single dot display. A single segment will be lit to indicate the input readings position on the scale. When scaling the display use the `bAr_` and `bAr^` functions e.g. `bAr_ = 0` and `bAr^ = 100` will give a bargraph with the bottom segment lit at a 7 segment display reading of `0` and the top segment lit with a 7 segment display reading of `100`. Note: this could also be set up as a centre zero single dot display by entering a negative value and positive value. e.g. `bAr_ = -100`, `bAr^ = 100`.

- **d.dot** - double dot display. Two segments will be lit to indicate the input reading position on the scale. The reading should be taken from the middle of the two segments. When scaling the display use the **bAr<sub>-</sub>** and **bAr<sup>-</sup>** functions e.g. **bAr<sub>-</sub> = 0** and **bAr<sup>-</sup> = 100** will give a bargraph with the bottom two segments lit at a 7 segment display reading of **0** and the top two segments lit with a 7 segment display reading of **100**. Note: this could also be set up as a centre zero double dot display by entering a negative value and positive value. e.g. **bAr<sub>-</sub> = -100**, **bAr<sup>-</sup> = 100**.
- **C.bAr** - centre bar display. The display will be a solid bargraph but will have its zero point in the middle of the display. If the seven segment display value is positive the bargraph will rise. If the seven segment display value is negative then the bargraph will fall. When scaling the display use the **bAr<sub>-</sub>** and **bAr<sup>-</sup>** functions e.g. **bAr<sub>-</sub> = 0** and **bAr<sup>-</sup> = 100** will give a bargraph with all the bottom half segments lit at a 7 segment display reading of **-100** and all the top segments lit with a 7 segment display reading of **100**.
- **r.dot** - modulus or wrap around single dot bargraph. This mode of operation allows the bargraph to wrap around the limits set by the **bAr<sub>-</sub>** and **bAr<sup>-</sup>** functions by dividing the 7 segment display by the modulus (the modulus is the difference between 0 and **bAr<sup>-</sup>**) and displaying the remainder. For example if **bAr<sub>-</sub>** is set to **0** and **bAr<sup>-</sup>** is set to **10** then in other bargraph modes when the 7 segment display reads a value such as **25** the bargraph would be stuck at the high limit of its travel since it cannot go beyond **10**. In **r.dot** mode the display will wrap around at **10** then continue up the bar again and will be at the midpoint of the bargraph when the 7 segment display shows **25** (as it would for a 7 segment display of **15**, **35**, etc.). In this example for a 7 segment display of **25** the value of 25 is divided by the modulus value of 10 in this example and the remainder displayed i.e. 10 goes into 25 twice with the remainder of 5 and so a bargraph position of 5 is displayed. This mode will operate on both vertical and circular bargraph type displays.

## 5.15 Digital output option mode

Display: **d90P**  
 Range: **bcd**, **b.SCL**, **b, n** or **b, n2**  
 Default Value: **b, n2**

Seen only with the 16 bit digital output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted. Selections available are: **b, n2** (signed binary) i.e. -32767 to 32767, **b, n** (unsigned binary) i.e. 0 to 65535, **b.SCL** (scaled binary, see **d, 9<sub>-</sub>** and **d, 9<sup>-</sup>** below), **bcd** (binary coded decimal) i.e. up to four BCD numbers.

## 5.16 Digital output option polarity

Display: **d9.OP**  
 Range: **Ri 0** or **RH, 1**  
 Default Value: **Ri 0**

Seen only with the 16 bit digital output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted. Selections available are: **Ri 0**

(active low i.e. logic 1 = 0V output, logic 0 = +V output) or **AH**, (active high i.e. logic 1 = +V output, logic 0 = 0V output).

## 5.17 Digital output option BCD start position

**Display:** **bcd Start**  
**Range:** Any display value  
**Default Value:** **0**

Seen only with the 16 bit digital output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted. This function affects BCD mode only and determines the number of digits to skip when outputting from the display. As the output is 16 bit it can output up to 4 BCD numbers. Select from **0** to number of display digits minus 4. e.g. for a 6 digit display you may select **0** to **2**, if **2** is selected then the four left most digits will be output, if set to **0** then the four right most digits will be output.

## 5.18 Digital output option low value

**Display:** **d, 9-**  
**Range:** Any display value  
**Default Value:** **0**

Seen only with the 16 bit digital output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted. Accepts any valid display value. Determines the low scaling point for the **b.SCL** mode and has no effect on other modes. See example which follows in 5.19.

## 5.19 Digital output option high value

**Display:** **d, 9~**  
**Range:** Any display value  
**Default Value:** **1000**




Seen only with the 16 bit digital output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted. Determines the high scaling point for the **b.SCL** mode and has no effect on other modes.

### Example:

If **d, 9-** is set to **0** and **d, 9~** is set to **65535** ( $2^{16} - 1$ ) then the retransmission will not be scaled i.e. a display of **2** will cause a retransmission of 2. If **d, 9~** is now changed to **32767** ( $2^{15} - 1$ ) then a display of **2** will cause a retransmission of 4 (note: rounding may occur on retransmission).

## 5.20 Analog output option low value

**Display:** `FEE_`  
**Range:** Any display value  
**Default Value:** `0`




Seen only when analog retransmission option fitted. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted for wiring details and link settings. Displays and sets the analog retransmission (4–20mA, 0–1V or 0–10V, link selectable) output low value (4mA or 0V) in displayed engineering units. To set the analog output low value go to the `FEE_` function and use the  or  push buttons to set the required value then press  to accept this selection.

### Example:

If it is required to retransmit 4mA when the display indicates `0` then select `0` in this function using the  or  button.

## 5.21 Analog output option high value

**Display:** `FEE^`  
**Range:** Any display value  
**Default Value:** `1000`

Seen only when analog retransmission option fitted. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when this option is fitted for wiring details and link settings. Displays and sets the analog retransmission (4–20mA, 0–1V or 0–10V, link selectable) output high display value (20mA, 1V or 10V) in displayed engineering units. To set the analog output high value go to the `FEE^` function and use the  or  push buttons to set the required value then press  to accept this selection.

### Example:

If it is required to retransmit 20mA when the display indicates `50` then select `50` in this function using the  or  button.

## 5.22 Second analog output option low value

**Display:** `FEE_ [h2`  
**Range:** Any display value  
**Default Value:** `0`

See `FEE_` function 5.20 for description of operation.



## 5.23 Second analog output option high value

Display: **FEC7 CH2**  
Range: Any display value  
Default Value: **1000**

See **FEC7** function 5.21 for description of operation.

## 5.24 Display rounding

Display: **drnd**  
Range: **1** to **5000**  
Default Value: **1**



Displays and sets the display rounding value. This value may be set to 1 - 5000 displayed units. Display rounding is useful for reducing the instrument resolution without loss of accuracy in applications where it is undesirable to display to a fine tolerance. To set the display rounding value go to the **drnd** function and use the  or  push buttons to set the required value then press **F** to accept this selection.

### Example:

If set to **10** the display values will change in multiples of 10 only i.e. display moves from **10** to **20** to **30** etc.



## 5.25 Decimal point

Display: **dCPE**  
Range: **0**, **0.1** etc.  
Default Value: **0**

Displays and sets the decimal point. By pressing the  or  pushbutton at the **dCPE** function the decimal point position may be set. The display will indicate as follows: **0** (no decimal point), **0.1** (1 decimal place), **0.02** (2 decimal places), **0.003** (3 decimal places) and **0.0004** for display with more than 4 digits. Note if the decimal point is altered the display will need to be recalibrated and alarm etc. settings checked.

## 5.26 Digital filter

Display: **FLtr**  
Range: **0** to **8**  
Default Value: **2**

Displays and sets the digital filter value. Digital filtering uses a weighted average method of determining the display value and is used for reducing display value variation due to short term interference. The digital filter range is selectable from **0** to **8**, where **0** = none and **8** = most filtering. Use  or  at the **FLtr** function to alter the filter level if required. Note that the

higher the filter setting the longer the display may take to reach its final value when the input is changed, similarly the relay operation and any output options will be slowed down when the filter setting is increased. To set the digital filter value go to the **Filter** function and use the **▲** or **▼** push buttons to set the required value then press **F** to accept this selection.

## 5.27 Display unit

Display: **di SP unit**  
 Range: **NONE °C °F .°C or F**  
 Default Value: **NONE**

Display unit - When used to measure temperature certain temperature display unit characters can be selected to appear on the display. Choices are:

**NONE** gives no display units e.g. a display such as **2345**

**°C** - gives **°C** display unit e.g. **45 °C**

**°F** - gives **°F** display unit e.g. **90 °F**

**°** - gives **°** display unit e.g. **123 °**

**°C** - gives **°C** display unit e.g. **45.2°C**

**F** - gives **F** display unit e.g. **237F**

Note that if a temperature display is selected the unit will take one or two of the available display digits, this will limit the maximum value which can be displayed. If the number becomes too large to display then an error message **-or-** will appear on the display.

## 5.28 First calibration scaling point

Display: **CAL 1**  
 Range: Any display value  
 Default Value: **0**

First scaling point for 2 point calibration scaling - See “Calibration” chapter, section 6.1.

## 5.29 Second calibration scaling point

Display: **CAL 2**  
 Range: Any display value  
 Default Value: **1000**

Second scaling point for 2 point calibration scaling - See “Calibration” chapter, section 6.1.

### 5.30 Calibration offset

**Display:** **CAL OFFt**  
**Range:** Any display value  
**Default Value:** n/a

Calibration offset - See section 6.3.

### 5.31 Zero range

**Display:** **ZERO RANGE**  
**Range:** Any display value or **OFF**  
**Default Value:** **OFF**

Zero range limit value - see section 6.4.

### 5.32 Calibration zero

**Display:** **CAL ZERO**  
**Range:** n/a  
**Default Value:** n/a

Zero point calibration for **ZERO RANGE** function - see section 6.5.

### 5.33 4mA input scale

**Display:** **USER En4**  
**Range:** Any display value  
**Default Value:** n/a

4mA input scale value, use only as an alternative to **CAL 1** and **CAL 2** calibration - See “Calibration” chapter, section 6.2.

### 5.34 20mA input scale

**Display:** **USER En20**  
**Range:** Any display value  
**Default Value:** n/a

20mA input scale value, use only as an alternative to **CAL 1** and **CAL 2** calibration - See “Calibration” chapter, section 6.2.

### 5.35 Uncalibrate

Display: **UCAL**

Range: n/a

Default Value: n/a

Uncalibrate, resets calibration - required only when a calibration problem occurs and it is necessary to clear the calibration memory. At the **UCAL** function press the **▲** and **▼** buttons simultaneously. The message **CAL CLR** should be seen to indicate that the calibration memory has been cleared.

### 5.36 Analog output PI control

Display: **rEc ctrl**

Range: **on** or **OFF**

Default Value: **OFF**

Analog output mode - seen only when analog output option is fitted. This function allows selection of **on** or **OFF** for PI control analog output. If set to **OFF** the analog output operates as a retransmission output and uses the functions described in this chapter. If set to **on** the analog output operates as a PI control output. Note if the dual analog output option is fitted only the first of these outputs can be configured for PI control.

When this function is set to **on** the following associated functions will appear: **C.SET**, **C.SPAN**, **C.P9**, **C.P0**, **C.I9**, **C.L.H**, **C.L.L** and **FEE SPAC**. These functions are not detailed in this manual. Refer to the separate "PM4 Panel Meter Optional Output Addendum" booklet for description of the analog PI control functions and wiring details.

### 5.37 **P** button function

Display: **Pbut**

Range: **NONE.H**, **.Lo.H**, **Lo.tARE**, **.ZEFO**, **P.SET** or **O.Put**

Default Value: **NONE**

**P** button function - a only applicable models with front panel **P** buttons. The **P** button may be set to operate some of functions also available via the remote input, see **r.I NP** below for a description of these functions. The **P** button is located at the front of 5 or 6 digit LED models and bargraph models. If both the remote input and **P** button function are operated simultaneously the **P** button will override the remote input. The functions below are as described in the **r.I NP** function below. Functions available are: **NONE.H**, **.Lo.H**, **Lo.tARE**, **.ZEFO**, **P.SET** or **O.Put**. Note: To prevent accidental operation of the **P** button in the **tARE** or **.ZEFO** functions it is necessary to hold the button in for 2 seconds to perform the selected operation.

## 5.38 Remote input function

Display: **FLNP**  
Range: **NONE . P.HLd . d.HLd . H<sub>i</sub> . Lo . H<sub>i</sub> Lo . tARE . ZER0 . SP.Ac . No.Ac .  
CAL.S . P.SET . dULL** or **Q.Put**  
Default Value: **NONE**

Remote input function - When these remote input terminals are short circuited, via a switch, relay, keyswitch etc. the instrument will perform the selected remote input function. A message will flash to indicate which function has been selected when the remote input pins are short circuited. The remote input functions are as follows:

**NONE** - no remote function required i.e. activating the remote input has no effect.

**P.HLd** - peak hold. The display will show the peak value (highest positive value) only whilst the remote input terminals are short circuited i.e. the display value can rise but not fall whilst the input terminals are short circuited. The message **P.HLd** will appear briefly every 8 seconds whilst the input terminals are short circuited to indicate that the peak hold function is active.

**d.HLd** - display hold. The display value will be held whilst the remote input terminals are short circuited. The message **d.HLd** will appear briefly every 8 seconds whilst the input terminals are short circuited to indicate that the display hold function is active.

**H<sub>i</sub>** - peak memory. The peak value stored in memory will be displayed if the remote input terminals are short circuited, if the short circuit is momentary then the display will return to normal measurement after 20 seconds. If the short circuit is held for 2 to 3 seconds or the power is removed from the instrument then the memory will be reset.

**Lo** - valley memory. The minimum value stored in memory will be displayed. Otherwise operates in the same manner as the **H<sub>i</sub>** function described above.

**H<sub>i</sub> Lo** - toggle between **H<sub>i</sub>** and **Lo** displays. This function allows the remote input to be used to toggle between peak and valley memory displays. The first operation of the remote input will cause the peak memory value to be displayed, the next operation will give a valley memory display. **PH<sub>i</sub>** or **PLo** will flash before each display to give an indication of display type.

**tARE** - display tare. Short circuiting the remote input pins momentarily will allow toggling between nett and gross values (shown as **NETt** and **GR0S**). If the remote input is short circuited for approx. 2 seconds the display will be tared and will show zero. The tare will be lost if power is removed.

**ZER0** - display zero. Zeroes the display in same manner as the tare function except that the zero is not lost when power is removed and the display will zero as soon as the remote input is shorted. When the **ZER0** operation is used the gross value cannot be recalled and the input at the time of the **ZER0** operation will become the new zero point.

**SP.Ac** - setpoint access only. This blocks access to any functions except the alarm setpoint functions unless the remote input pins are short circuited or entry is made via **CAL** mode or if the **ACCS** function is set to **ALL**.

**No.Ac** - no access. This blocks access to all functions unless the remote input pins are short circuited or entry is made via **CAL** mode or if the **ACCS** function is set to **ALL**.

**CAL.5** - calibration select. The remote input can be used to select between calibration scaling values. Two sets of calibration values can be entered in the PM4, one set with the remote input terminals open circuit and another set with the remote input terminals short circuit to ground. The remote input can then be used to switch between one set and the other. For example: With the remote input open circuit a 4–20mA input can be scaled (using **CAL 1** and **CAL2** or **USER EN4** and **USER EN4**) to read **0** to **100** over the 4–20mA range. With the remote input short circuit to ground the scaling can be repeated using figures of **0** to **500** for the 4–20mA range. The remote input can be used to switch between ranges. In this example the first scaling could represent a percentage figure and the second scaling could represent the actual process units (litres, kg, volts etc). Note: Alarm settings will not change when changing between calibrations scales. i.e. Only one set of alarm functions can be made and the alarm relay will operate from those set values no matter which calibration scale is being viewed at the time. The **DISP UNIT**, **dCPE** and **ZERO RANGE** functions can be individually set for each channel. If **P.SET** is used only one preset value can be used but only the channel displayed at the time is affected. Note; using different **dCPE** settings between channels will affect the preset and alarm setpoint values e.g. a preset of **25** on a channel with **dCPE = 0** will become **2.5** on a channel with **dCPE = 0.1**.

**P.SET** - preset value. The remote input can be used to force the display to the preset value, this preset value is set at the **P.SET** function.

**dULL** - display brightness control. The remote input can be used to change the display brightness. When this mode is selected the display brightness can be switched, via the remote input terminals, between the brightness level set at the **brgt** function and the brightness level set at the **dULL** function.

**0.Put**- serial “print” output - applicable only when the serial output option is fitted - allows the remote input to be used to initiate a single serial string output. The value output can be set to the live input value, the display value or one of the appropriate remote input functions. If a remote input function is selected such as **Hi, Lo** then in addition to the serial output function (**SEFL**) being selected as **Hi, Lo** a remote input (**FI NP**) or the **P** button (**Pbut**) function must also be set to **Hi, Lo**. The serial output will be a single string beginning with a start of text character <STX> and ending with a carriage return <CR> the value will occur between these two control characters. In the case of a **Hi, Lo** operation the high value will be separated from the low value by a comma. e.g.:

<STX>Hi value, Lo value<CR>.

The transmitted string is in standard ASCII format. The functions required for this “print” output command are:

**Pbut** or **FI NP** - one of these functions must be set to **0.Put**. When the selected remote input is shorted to ground or the **P** button is pressed a single serial string of the value selected will be transmitted.

**0.Put** - this function must be set to **POLL**. When set to **POLL** the instruments serial communications can operate as either a “print” output or in the conventional polling mode.

**SEFL** - this function sets the value to be transmitted when using “print” output operation. The options are:

**L, UE** (live reading), the value sent will be the live input value determined from the calibration scaling and the level of the electrical input from the load cell or sensor.

- tARE** (tare), the value sent will follow the tared value when a remote input or **P** button has been used to tare the display.
- P.HLd** (peak hold), the value sent will be the peak value whilst the peak hold operation is in progress i.e. When a remote input is being used to cause a peak hold display. The value will be reset when the **P.HLd** remote input is deactivated.
- d.HLd** (display hold), the value sent will be the held display value whilst the display hold operation is in progress i.e. When a remote input is being used to cause a display hold. The value will be reset when the **d.HLd** remote input is deactivated.
- H**, (peak memory), the value sent will be the peak value in memory. This can be reset by activating the **H**, remote input or **P** button for 2 seconds or by removing power to the instrument.
- Lo** (valley memory), the value sent will be the lowest value in memory. This can be reset by activating the **Lo** remote input or **P** button for 2 seconds or by removing power to the instrument.
- d: SP** (display value), the value transmitted will be whatever value is on the display at the time of a “print” operation.
- H, Lo** (peak, valley memory), the values sent will be the peak value in memory followed by a comma followed by the lowest value in memory. These can be reset by activating the **H, Lo** remote input or **P**

### Example:

To make the serial “print” output send the peak held value using remote input as the peak hold remote input and the **P** button as the “print” input:

1. Set the **r: NP** function to **P.HLd**
2. Set the **Pbut** function to **O.Put**
3. Set the **O.Put** function to **POLL**
4. Set the **SEFL** function to **P.HLd**

Whilst the remote input terminal is short circuited to the GND terminal the display will show the peak held value. When the **P** button is pressed a single serial string showing the peak held value will be transmitted.

## 5.39 Nett flash inhibit

Display: **NETt FLSH**  
 Range: **on** or **OFF**  
 Default Value: **OFF**

Nett value display mode - the nett value is only seen when the remote input **r: NP** or **P** button **Pbut** function is set to **tARE** and can therefore toggle between gross and nett displays. The **NETt FLSH** function can be set to on or **OFF**. If set to **on** then the message **NETt** will flash briefly approximately every 6 seconds when the operator toggles to a nett display to remind the operator that a nett value is being viewed. If set to **OFF** then the message **NETt** will flash briefly once only when the operator toggles to the nett value.

## 5.40 Access mode

Display: **ACCS**  
Range: **OFF**, **EASY**, **NONE** or **ALL**  
Default Value: **OFF**

Access mode - the access mode function **ACCS** has four possible settings namely **OFF**, **EASY**, **NONE** and **ALL**. If set to **OFF** the mode function has no effect on alarm relay operation. If set to **EASY** the “easy alarm access” mode will be activated. Refer to “Easy alarm relay adjustment access facility” page 17. If set to **NONE** there will be no access to any functions via **FUNC** mode, entry via **CAL** mode must be made to gain access to alarm and calibration functions. If set to **ALL** then access to all functions, including calibration functions, can be gained via **FUNC** mode.

## 5.41 Setpoint access mode

Display: **SPAC**  
Range: **A 1**, **A 1-2** etc.  
Default Value: **A 1**

Setpoint access - seen only if more than 1 relay fitted. Sets the access via **FUNC** mode and “easy alarm access” mode to the alarm relay setpoints. The following choices are available:

**A 1** - Allows setpoint access to alarm 1 only.

**A 1-2** - Allows setpoint access to alarms 1 and 2 only.

**A 1-3** - Allows setpoint access to alarms 1, 2 and 3 etc. up to the maximum number of relays fitted.

The remote input function (**FINP**) must be set to **SPAC** for this function to operate. Note: Only the setpoints which have been given a value will be accessible e.g. if **A 1H** is set to **OFF** then there will be no access to the **A 1H** function when **SPAC** is used.

## 5.42 Square root mode

Display: **Sqrt**  
Range: **on** or **OFF**  
Default Value: **OFF**

Square root - selects the square root scaling to **on** or **OFF**. When set to **on** a square root function is applied to the input. When set to **OFF** the calibration is a linear function. When the square root facility is used the scaled displayed value follows the square root of the percentage of the full scale input value. The upper and lower input limits are set as normal as are the values to be displayed at these limits.

Note: It is essential that the display is rescaled, using **CAL 1** and **CAL 2** or **USER E n4** and **USER E n20**, whenever the square root function is turned on or off. The **CAL OFSt** function cannot be used when the **Sqrt** function is set to **on**.

### Example:

For a 4–20mA input if you wish to display 0 at 4mA and 1000 at 20mA the square root function will calculate as follows:

At 20mA (100%) the display will be **1000** i.e.  $\sqrt{1} \times 1000$ .  
 At 16mA (75%) the display will be **866** i.e.  $\sqrt{0.75} \times 1000$ .  
 At 12mA (50%) the display will be **707** i.e.  $\sqrt{0.5} \times 1000$  and so on.

### 5.43 Alarm relay operation mode

**Display:** **A 1.A2** etc.  
**Range:** **L, UE, TARE, P.HLd, d.HLd, H, Lo** or **d: SP**  
**Default Value:** **L, UE**

Alarm relay operation mode for relays 1, 2 etc. The following choices are available for alarm operation mode:

**L, UE** - live input mode. The alarm relay operation will always follow the electrical input at that time irrespective of the 7 segment display value. e.g. assume the remote input is set to **TARE** and **A 1H** is set to **100**. If the instrument is tared at a display reading of **30** then the alarm will now activate at a display reading of **70**. Note that if a remote input or **P** button **ZERO** operation has been carried out the above example does not apply i.e. for the above if the display was zeroed rather than tared at a display of **30** then the relay will still activate at a display of **100**, this is due to the fact that the zero operation permanently shifts the live calibration.

**TARE** - tare mode. The alarm relay operation will follow the tare function. e.g. in the example above (**d: SP**) if **A 1** is set to **TARE** then the alarm would activate at a display reading of **100** (the setpoint value) rather than **70**.

**P.HLd** - peak hold mode. If the peak hold mode is used and the remote input is set to peak hold (**P.HLd**) then once the peak display goes above any alarm high setpoint the alarm relay will activate and will not de-activate until the peak hold is released and the display value falls below the setpoint value.

**d.HLd** - display hold mode. If the display hold mode is used and the remote input is set to display hold (**d.HLd**) then the alarm relay will be held in its present state (activated or de-activated) until the display hold is released and the display is free to change.

**H** - peak (max.) memory mode. If the peak memory mode is used and the remote input is set to peak memory (**H**) then the alarm will be activated if the peak memory value is above the high setpoint value. The alarm will not de-activate until the memory is reset.

**Lo** - valley (min.) memory mode. If the valley memory mode is used and the remote input is set to valley memory (**Lo**) then the alarm relay will be activated if the valley memory value is below the low setpoint value. The alarm will not de-activate until the memory is reset.

**d: SP** - display mode. If the live display mode is used then the alarms will operate purely on the display value at the time i.e. if the display is showing above high setpoint or below the low setpoint value then the alarm relay will activate.

## 5.44 Bargraph display operation mode

Display: **BAR**  
Range: **L, UE, TARE, PHLD, d.HLD, H, Lo** or **di SP**  
Default Value: **L, UE**

The following choices are available for bargraph display mode:

**L, UE** - live input mode. The bargraph display will always follow the electrical input at that time irrespective of the 7 segment display value. For example if the remote input is set for peak hold operation then when the remote input is closed the 7 segment display will only show the peak value but the bargraph will be free to move up and down to follow the live input. Note that the **L, UE** mode does not follow the electrical input if a remote input or **P** button **ZERO** operation has been undertaken. This is due to the fact that the **ZERO** operation shifts the display calibration.

**TARE** - tare mode. The bargraph display will follow the tare function i.e fall to zero when the instrument is tared. If the remote input toggles the 7 segment display to show gross (**GRS**) then the 7 segment display will change to show the gross value but the bargraph will not respond (see **L, UE** for alternative operation.)

**PHLD** - peak hold mode. The bargraph (and 7 segment display) will indicate the peak value only whilst the peak value function is operated via a contact closure on the remote input i.e. the bargraph and 7 segment display can rise but not fall whilst the remote input switch is closed. When the remote input switch is opened the bargraph value will remain fixed i.e. it will not rise or fall, although the 7 segment display value will be free to alter. This peak bargraph reading can be cleared by closing the remote input switch for another operation or by temporarily removing power from the instrument. Note: In this mode the bargraph will show a zero reading until the remote input is operated for the first time after switch on.

**d.HLD** - display hold mode. The bargraph (and 7 segment display) value will be held whilst the remote input display hold switch is closed. When the switch is opened the bargraph value will remain fixed at the held value although the 7 segment display value will be free to alter. The held bargraph reading can be cleared by closing the remote input switch for another operation or by removing power from the instrument. Note: In this mode the bargraph will show a zero reading until the remote input is operated for the first time after switch on.

**H** - peak (max.) memory mode. With the peak remote input switch open the bargraph will indicate the peak value in memory i.e. the bargraph can rise but not fall. The bargraph can be reset by clearing the memory. The memory may be cleared either by closing the remote input switch for approximately 2 seconds or by temporarily removing power to the instrument.

**Lo** - valley (min.) memory mode. With the valley remote input switch open the bargraph will indicate the valley (min.) value in memory i.e. the bargraph can fall but not rise. The bargraph can be reset by clearing the memory. The memory may be cleared either by closing the remote input switch for approximately 2 seconds or by temporarily removing power to the instrument.

**di SP** - display mode. The bargraph display will follow whatever value is on the 7 segment display. For example if the remote input is to **TARE** then the 7 segment and bargraph will indicate the tared value and both will also be changed if the remote input toggles the displays between **NET** and **GRS**. If the **BAR** function had been set to **TARE** then the bargraph would not respond to the **GRS** toggle.

## 5.45 Analog/digital/serial operation mode

Display: **rEC** or **rEC2** or **d9.OP** or **SEFL**  
Range: **L, UE, TARE, PHLD, d.HLD, H, Lo** or **d: SP**  
Default Value: **L, UE**

This section describes the operation modes available for the retransmission options **rEC** (analog retransmission) operation mode or **rEC2** (second analog retransmission) or **d9.OP** (digital output retransmission) or **SEFL** (serial retransmission). The following choices are available:

**L, UE** - live input mode. The retransmission will follow the electrical input and will not necessarily follow the 7 segment or bargraph display. For example if the remote input is set for peak hold operation then when the remote input is closed the 7 segment display will only show the peak value but the retransmission will be free to change to follow the electrical input. Note that the **L, UE** mode does not follow the electrical input if a remote input or **P** button **ZERO** operation has been undertaken. This is due to the fact that the **ZERO** operation shifts the display calibration.

**TARE** - tare mode. The retransmission value will tare (fall to zero) along with 7 segment display when the remote input tare function is operated. If the remote input toggles the 7 segment display to show gross (**GR05**) then the 7 segment display will change to show the gross value but the retransmission will not respond (see **L, UE** for alternative operation).

**PHLD** - peak hold mode. The 7 segment display and retransmission value will indicate the peak value only whilst the peak value function is operated via a contact closure on the remote input i.e. the 7 segment display and retransmission can rise but not fall whilst the remote input switch is closed. When the remote input switch is opened the retransmission value will remain fixed i.e. it will not rise or fall, although the 7 segment display value will be free to alter. This peak retransmission output can be cleared by closing the remote input switch for another operation or by removing power from the instrument. Note: In this mode the retransmission will show a zero reading until the remote input is operated for the first time after switch on.

**d.HLD** - display hold mode. The 7 segment display and retransmission value will be held whilst the remote input display hold switch is closed. When the switch is opened the retransmission value will remain fixed at the held value although the 7 segment display value will be free to alter. The held retransmission output can be cleared by closing the remote input switch for another operation or by removing power from the instrument. Note: In this mode the bargraph will show a zero reading until the remote input is operated for the first time after switch on.

**H** - peak (max.) memory mode. With the peak remote input switch open the retransmission will indicate the peak value in memory i.e. the retransmission output can rise but not fall. The retransmission output can be reset by clearing the memory. The memory may be cleared either by closing the remote input switch for approximately 2 seconds or by removing power to the instrument.

**Lo** - valley (min.) memory mode. With the valley remote input switch open the retransmission will indicate the valley (min.) value in memory i.e. the retransmission output can fall but not rise. The retransmission output can be reset by clearing the memory. The memory may be cleared either by closing the remote input switch for approximately 2 seconds or by removing power to the instrument.

**d: SP** - display mode. The retransmission output will follow whatever value is on the 7 segment display. For example if the remote input is set to **TARE** then the 7 segment and retransmission

output will indicate the tared value and both will also be changed if the remote input toggles the displays between **NETT** and **GR05**. If the **REC** or **d90P** function had been set to **SAFE** then the retransmission output would not respond to the **GR05** toggle.

## 5.46 Low overrange visual warning limit value

**Display:** **Lo di SP**  
**Range:** Any display value or **OFF**  
**Default Value:** **OFF**

Low overrange limit value - the display can be set to show an overrange message if the display value falls below the **Lo di SP** setting. For example if **Lo di SP** is set to **50** then once the display reading falls below **50** the message **-or-** will flash on and off or the display value will flash on and off instead of the normal display units (see **di SP** function 5.48). This message can be used to alert operators to the presence of an input which is below the low limit. If this function is not required it should be set to **OFF** by pressing the **▲** and **▼** buttons simultaneously at this function.

## 5.47 High overrange visual warning limit value

**Display:** **Hi 9H di SP**  
**Range:** Any display value or **OFF**  
**Default Value:** **OFF**

High overrange limit value - the display can be set to show an overrange message if the display value rises above the **Hi 9H di SP** setting. For example if **Hi 9H di SP** is set to **1000** then once the display reading rises above **1000** the message **-or-** will flash on and off or the display value will flash on and off instead of the normal display units (see **di SP** function 5.48). This message can be used to alert operators to the presence of an input which is above the high limit. If this function is not required it should be set to **OFF** by pressing the **▲** and **▼** buttons simultaneously at this function.

## 5.48 Display visual warning flashing mode

**Display:** **di SP**  
**Range:** **FLASH** or **-or-**  
**Default Value:** **FLASH**

Display overrange warning flashing mode - this function is used in conjunction with the **Lo di SP** and **Hi 9H di SP** functions. The **di SP** function can be set to **FLASH** or **-or-**. If the display warning value set at the **Lo di SP** or **Hi 9H di SP** function is exceeded and the **di SP** function is set to **FLASH** then the display value will flash on and off every second as a visual warning. If the display warning value set at the **Lo di SP** or **Hi 9H di SP** function is exceeded and the **di SP** function is set to **-or-** then the **-or-** message will flash on and off once a second as a visual warning. The warning flashes will cease and the normal display value will be seen when the value displayed is higher than the low limit and lower than the high limit.

## 5.49 Baud rate for optional serial communications

Display: **baud**  
Range: **300 . 600 . 1200 . 2400 . 4800 . 9600 . 19.2** or **38.4**  
Default Value: **9600**

Set baud rate - seen only with serial output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when optional outputs are fitted. Select from **300 . 600 . 1200 . 2400 . 4800 . 9600 . 19.2** or **38.4** baud.

## 5.50 Parity for optional serial communications

Display: **Prty**  
Range: **NONE . EVEN** or **odd**  
Default Value: **NONE**

Set parity - seen only with serial output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when optional outputs are fitted. Select parity check to either **NONE** , **EVEN** or **odd**.

## 5.51 Output mode for optional serial communications

Display: **O.Put**  
Range: **di SP . Cont . POLL** , **R.buS** or **ā.buS**  
Default Value: **Cont**

Set serial interface mode - seen only with serial output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when optional outputs are fitted. . Allows user to select the serial interface operation as follows:

**di SP** - sends image data from the display without conversion to ASCII.

**Cont** - sends ASCII form of display data at a rate typically 90% of the sample rate.

**POLL** - controlled by computer or PLC as host. Host sends command via RS232/485 and instrument responds as requested.

**R.buS** - is a special communications mode used with Windows compatible optional PC download software. Refer to the user manual supplied with this optional software.

**ā.buS** - Modbus RTU protocol.

## 5.52 Instrument address for optional serial communications

Display: **Addr**  
Range: **0** to **31**  
Default Value: **0**

Set unit address for polled (**POLL**) mode (**0** to **31**) - seen only with serial output option. Refer to the separate “PM4 Panel Meter Optional Output Addendum” booklet supplied when optional

outputs are fitted. Allows several units to operate on the same RS485 interface reporting on different areas etc. The host computer or PLC may poll each unit in turn supplying the appropriate address. The unit address ranges from 0 to 31 (DEC) but is offset by 32 (DEC) to avoid clashing with ASCII special function characters (such as <STX> and <CR>). Therefore 32 (DEC) or 20 (HEX) is address 0, 42 (DEC) or 2A (HEX) is address 10.

### 5.53 Serial mode for optional serial communications

Display: **SEFL**  
Range: **L, uE, tARFE, P.HLd, d.HLd, H, .Lo, H, Lo** or **d! SP**  
Default Value: **L, uE**

Serial retransmission mode - seen only with serial output option - applies only when **O.Put** function set to **Cont**. Refer to **rEC** or **rEC2** or **d9.OP** or **SEFL** function 5.45 on for function description. The **H, Lo** selection in this functions allows both the peak and valley memories to be transmitted. The peak value will be transmitted followed by a space then the valley value.

### 5.54 Returning to normal measure mode

When the calibration has been completed it is advisable to return the instrument to the normal mode (where calibration functions are less likely to be tampered with). To return to normal mode, turn off power to the instrument, wait a few seconds and then restore power.

### 5.55 Error messages

**SPAN Err** - calibration span error. Live inputs used at **CAL 1** and **CAL 2** too close in value. Recalibrate using inputs further apart in value. If you are certain that the inputs are far enough apart but still see the **SPAN Err** message then ignore the message and continue with the two point calibration. At the end of the calibration check to see if the display calibration is correct and if not recalibrate using the same inputs.

**ZERO RANGE Err** - Zero range error. Caused by an attempt to zero the display outside the allowed range. See **ZERO RANGE** function.

**Unstable display** - if the display is not stable the usual cause is either that the input signal is unstable or that the calibration scaling was incorrectly attempted. If the calibration scaling was unsuccessful then uncalibrating the display at the **UCAL** function should return the display to stable readings but the previous calibration scaling values will be lost. If the display is still not stable after uncalibrating then check the input for stability and noise.

**Display shows “- - - -”** - this message indicates that the input signal is higher than the range selected. e.g. for an input set for 0-1V the “- - - -” message will be seen if the input signal goes much higher than 2V.

**Display shows -or-** - this message indicates either that the number is too big to display e.g. above **9999** on a 4 digit display or that the **d! SP** function has been set to **-or-** and either the **Lo d! SP** or **Hi 9H d! SP** limits have been exceeded.

**Display value flashes on and off** - this indicates that the **di SP** function has been set to **FLSH** and either the **Lo di SP** or **Hi GH di SP** limits have been exceeded.

**Display shows NO ACC** - this indicates that the **ACCS** function has been set to **NONE** or the **Fi NP** function has been set to **no.Ac** blocking entry to **FUNC** mode. Enter functions via **CAL** mode to gain entry to functions and if required change the **ACCS** or **Fi NP** function setting.

**Display shows NO SPAC** - this indicates that the **Fi NP** function has been set to **SP.Ac** blocking entry to alarm relay functions. Enter functions via **CAL** mode to gain entry to functions and if required change the **Fi NP** function setting.

## 6 Calibration

The instrument can be calibrated via a two point live input calibration method using functions **CAL 1** and **CAL 2**. For 4-20mA inputs only an alternative method allows display scaling without live inputs using the **USER En4** and **USER En20** functions. An offset calibration scaling adjustment using the **CAL OFFSt** function is available which allows the scaling to be adjusted by a fixed amount over the entire scale. Each of these methods and other calibration scaling function are described in this chapter.



In order to gain access to the calibration functions you must be in **CAL** mode, refer to the Chapter 5 which shows the method of entering **CAL** mode.

### 6.1 Live signal input calibration

**CAL 1** and **CAL 2** - The functions **CAL 1** and **CAL 2** are used together to scale the instruments display, values for both **CAL 1** and **CAL 2** must be set when using this scaling method. The **CAL 1** function sets the first calibration point for live input calibration. When using this method different signals inputs must be present at the input terminals for **CAL 1** and **CAL 2**. Note: **CAL 1** and **CAL 2** can be set independently.

The procedure for entering the first scaling point **CAL 1** is as follows:


- Ensure that an input signal is present at the input terminals, this will usually be at the low end of the signal range e.g. 4mA for a 4-20mA input.
- At the **CAL 1** function press **▲** and **▼** simultaneously then release them. The display will show the live input value. Do not be concerned at this stage if the live input display value is not what is required. It is important that the live input value seen is a steady value, if not then the input needs to be investigated before proceeding with the scaling.
- Press then release the **F** button. The display will indicate **SCL 1** followed by a value. Use the **▲** or **▼** button to change this value to the required display value at this input. e.g. if 4mA was input and the required display at 4mA was **0** then ensure **0** is entered at **SCL 1**. Press the **F** button to accept changes or the **P** button to abort the scaling. If the scaling has been accepted the **CAL End** message should be seen.

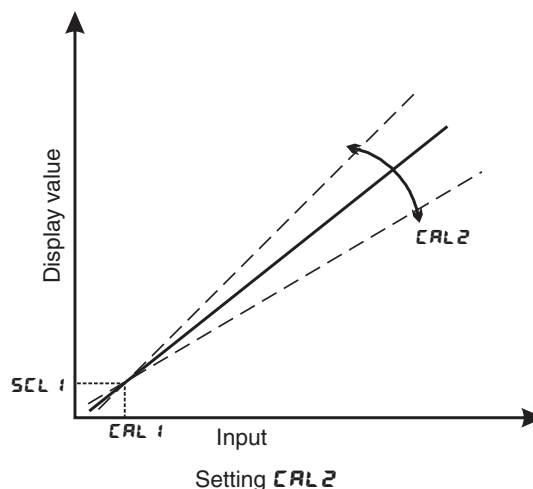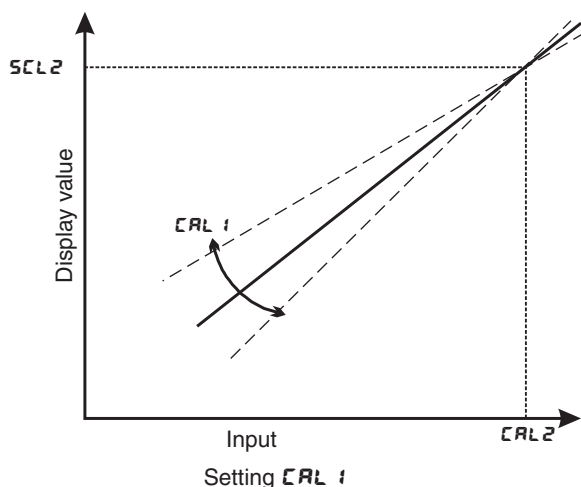

The procedure for entering the second scaling point **CAL2** is as follows:

- a. Ensure that an input signal is present at the input terminals, this will usually be at the high end of the signal range e.g. 20mA for a 4-20mA input. The change in input signal from the **CAL 1** input must be at least 10% of the input range full scale.
- b. At the **CAL2** function press **▲** and **▼** simultaneously then release them. The display will show the live input value. Do not be concerned at this stage if the live input display value is not what is required. It is important that the live input value seen is a steady value, if not then the input needs to be investigated before proceeding with the scaling.
- c. Press then release the **F** button. The display will indicate **SCAL2** followed by a value. Use the **▲** or **▼** button to change this value to the required display value at this input. e.g. if 20mA was input and the required display at 20mA was **500** then ensure **500** is entered at **SCAL2**. Press the **F** button to accept changes or the **P** button to abort the scaling. If the scaling has been accepted the **CAL End** message should be seen.

Example - Flow chart showing scaling using two live inputs

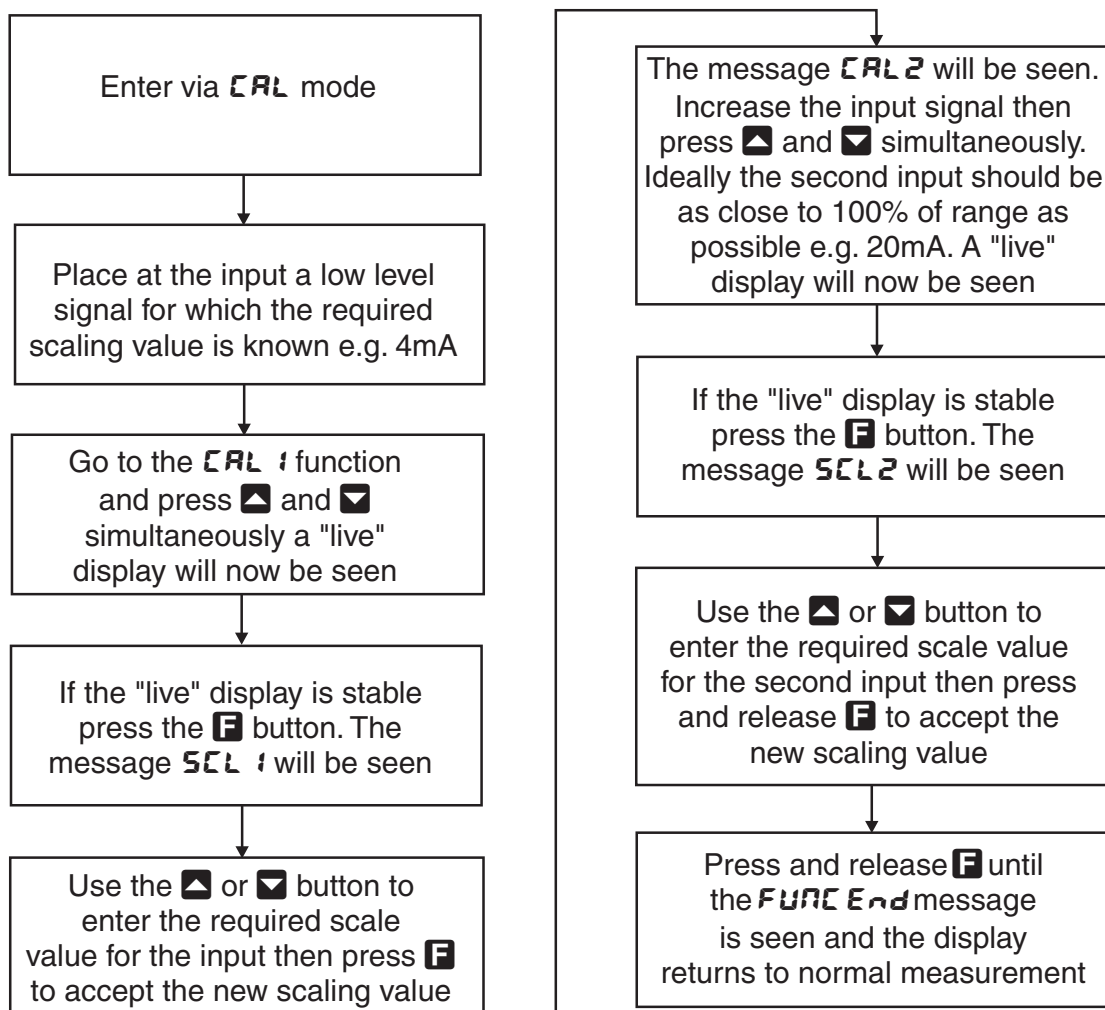

Note: If the "live" display at any scaling point is not stable then check the input signal for stability.

## 6.2 Alternative 4-20mA scaling

**USER En4** - 4mA input scaling without a live input - this calibration method can be used with 4-20mA inputs only. The instrument can be scaled for a 4-20mA input without a live input i.e. this is an alternative method to the **CAL 1** and **CAL 2** method of scaling. To perform the first point (**En4**) scaling simply press the **▲** and **▼** buttons simultaneously when the **USER En4** function is displayed. The display will now indicate a value. Use the **▲** or **▼** button to change this value to the display value required for a 4mA input. Press the **F** button to accept changes or the **P** button to abort the scaling. If the scaling has been accepted the **CAL End** message should be seen.

**USER En20** - 20mA input scaling without a live input - this calibration method can be used with 4-20mA inputs only. To perform the second point (**En20**) scaling simply press the **▲** and **▼** buttons simultaneously when the **USER En20** function has been reached. The display will now indicate a value. Use the **▲** or **▼** button to change this value to the display value required for a 20mA input. Press the **F** button to accept changes or the **P** button to abort the scaling. If the scaling has been accepted the **CAL End** message should be seen.

Note: the **USER En4** and **USER En20** method relies on the accuracy of the signal input. If the sensor output is found to have an offset use the **CAL OFSt** function to correct for the offset. If the slope of the sensor output is not correct then **CAL 1** and **CAL 2** methods will have to be used.

## 6.3 Offset calibration

**CAL OFSt** - Calibration offset - the calibration offset is a single point adjustment which can be used to alter the calibration scaling values across the entire measuring range without affecting the calibration slope. This method can be used instead of performing a two point calibration when a constant measurement error is found to exist across the entire range. To perform a calibration offset press the **▲** and **▼** buttons simultaneously at the **CAL OFSt** function. A “live” reading from the input will be seen, make a note of this reading. Press the **F** button, the message **SCLE** will now be seen followed by the last scale value in memory. Use the **▲** or **▼** button to adjust the scale value to the required display value for that input. For example if the “live” input reading was **50** and the required display value for this input was **70** then adjust the **SCLE** value to **70**. Press the **F** button to accept changes or the **P** button to abort the scaling. If the scaling has been accepted the message **OFSt End** should be seen. If the **ZERO RANGE Err** message is seen refer to the **ZERO RANGE** and **CAL ZERO** functions.

## 6.4 Zero range

**ZERO RANGE** - Zero Range - the zero range function allows a limit value to be set (in engineering units) above which the display will not zero i.e. if a zero operation is attempted via the **P** button, remote input or set zero function when the display value is greater than the zero range setting the display will refuse to zero and give a **ZERO RANGE Err** message (note that the **CAL OFSt** function is also affected by the **ZERO RANGE** setting). For example if the zero range setting is **10** the instrument will only respond to a zero operation if the display reading at the time is between **-10** and **10**. If the zero range function is not required it can be set to **OFF** by pressing the **▲** and **▼** buttons simultaneously at this function. When switched off the instrument can be zeroed no

matter what the display value. Note that the instrument keeps track of the value being zeroed at each operation, when the total amount zeroed from repeated operations becomes greater than the zero range value the instrument will reject the zero operation and a **ZERO RANGE Err** message will be seen. To allow a zero operation beyond this point either the **ZERO RANGE** function value will need to be raised or a new zero reference point introduced via the **CAL ZERO** function. If repeated zero operations are required the **ZERO RANGE** function should be set to **OFF** or alternatively the **SAFE** operation could be considered.

## 6.5 Zero range zero calibration

**CAL ZERO** - Zero range zero calibration - a **CAL ZERO** zero operation can be used to ensure that the display zero and the **ZERO RANGE** reference zero are at the same point after a calibration. After a calibration the **CAL ZERO** operation can also be used to select a zero point other than the display zero as the reference for the **ZERO RANGE** function. For example if the **CAL ZERO** operation is carried out with a display reading of **500** and a **ZERO RANGE** reading of **10** the zero range function will allow the display to zero only if the current display reading is between **490** and **510**. To perform a calibration zero press the **▲** and **▼** buttons simultaneously at the **CAL ZERO** function, a live reading will be seen, press the **F** button, the message **CAL ZERO End** should now be seen indicating that the instrument has accepted the zero point. Although the display reading will not change as a result of the calibration zero the input value on the display at the time of the operation will be the new zero reference point for the **ZERO RANGE** function.

## 6.6 Uncalibration

**UCAL** - Uncalibrate - used to set the instrument back to the factory calibration values. This function should only be used when calibration problems exist and it is necessary to clear the calibration memory. To clear the calibration memory press the **▲** and **▼** buttons simultaneously at the **UCAL** function. The message **CAL CLR** will be seen to indicate that the memory has cleared.

## 7 Setting up the relay PI controller

The Relay Proportional + Integral Controller can be made to operate in either pulse width control or frequency control mode via the **Rx OPER** function. Note that the **Rx OPER** function will not be seen until a value has been set for the low or high alarm e.g. for **R ILo** or **R IH**. The best results are usually achieved by initially configuring as a “Proportional Only” controller and then introducing the Integral functions when stable results are obtained.

Relay 1 and , if fitted, relay 2 can be set to operate in PI control mode. Any other relays fitted will only operate in normal, non PI operation. The “x” in the **Rx OPER** and other functions indicates the chosen relay i.e. for relay 1 the display will show **R 1 OPER**, **R 1 SP** etc. The **Rx OPER** function allows three choices of operating mode for the chosen relay, namely **Rx.AL**, **Rx.tP** and **Rx.Fr**. If **Rx.AL** is selected the chosen relay will operate as a setpoint relay whose operation is controlled by the **Rx Hi**, **RxLo** etc. settings and the PI control settings will not be seen. See the “Explanation of functions” chapter for details of operation when **Rx.AL** is selected. If **Rx.tP** is selected then the chosen relay will operate in pulse width control mode. If **Rx.Fr** is selected then the chosen relay will operate in the frequency control mode.


**Pulse width control** - operates by controlling the on to off time ratio of the relay. In a typical application this would be used to control the length of time for which a dosing pump is switched on during a control cycle i.e. the pump or other device will continuously operate for the length of time the relay is activated and will stop operating when the relay is de-activated.

**Frequency control** - operates by changing the rate at which the relay switches on and off. In a typical control application the frequency control operation is particularly suited for use when one shot dosing is used i.e. the pump or other device puts out a fixed dosing quantity for every pulse received.

### 7.1 Relay pulse width modulation control mode

To use pulse width modulation control **Rx.tP** must be selected at the **Rx OPER** function.


Pulse width control

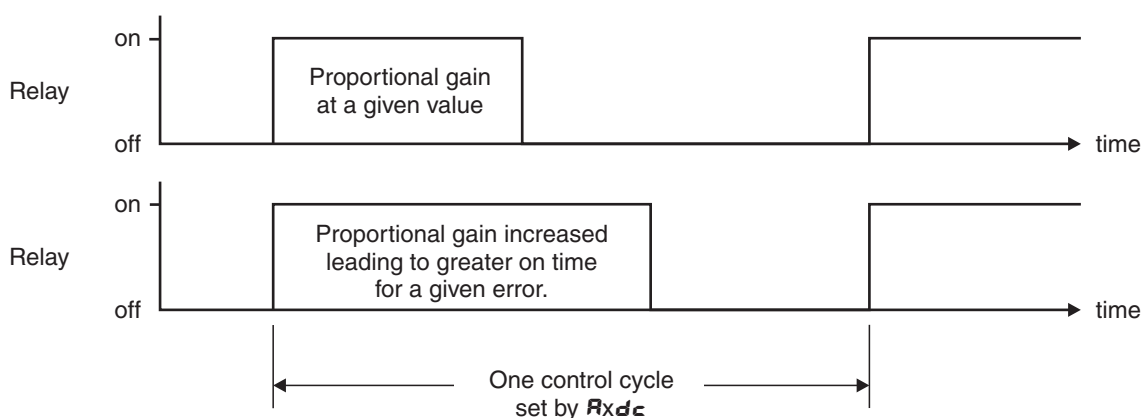

## 7.2 PI relay control setpoint

**Display:** ***Ax.SP***  
**Range:** Any display value  
**Default Value:** **0**

The control setpoint is set to the value in displayed engineering units required for the control process. The controller will attempt to vary the control output to keep the process variable at the setpoint. Note that the control setpoint value can be reached and adjusted via the “easy access” mode (see “Explanation of functions” chapter) if the **ACCS** function is set to **EASY**. This feature could be useful if the setpoint is to be frequently changed.

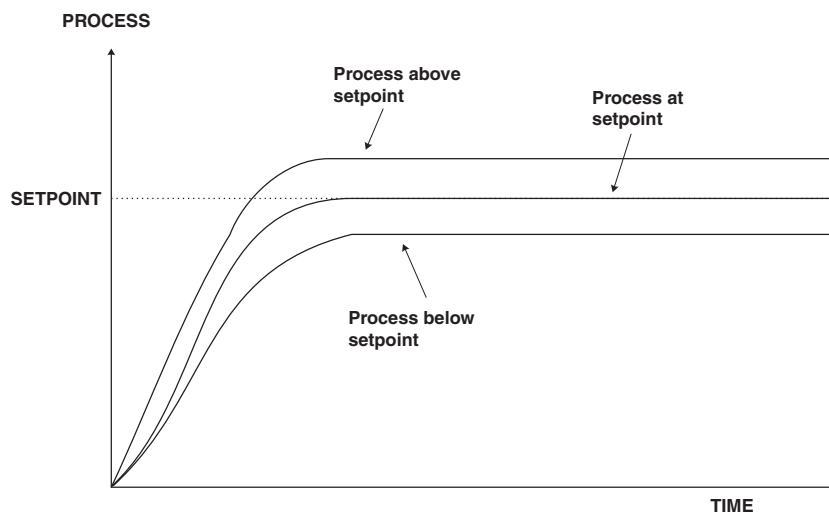

## 7.3 PI relay control span

**Display:** ***ctrl SPAN***  
**Range:** Any display value  
**Default Value:** **100**


The function of the control span is to define the limit to which the PI control values will relate. The control span value will be common to all control relays i.e. if more than one control relay output is being used then each of these relays operates from the same control span setting. The span value defines the range over which the input must change to cause a 100% change in the control output when the proportional gain is set to **1.000**. This function affects the overall gain of the controller and is normally set to the process value limits that the controller requires for normal operation. For example if the control setpoint (***Ax.SP***) is **70** and the ***ctrl SPAN*** is **20** and ***Ax.P9*** is set to **1.000** then an error of **20** from the setpoint will cause a 100% change in proportional control output. For example with ***Ax.SP*** at **70**, ***ctrl SPAN*** at **20**, ***Ax.P9*** at **1.000** and ***Ax.b5*** at **0.000** a display reading of **50** or lower (***Ax.SP*** minus ***ctrl SPAN***) the control output will be at 100% i.e. the relay will be on continuously. The control output will then gradually adjust the on/off time as the display value reaches the setpoint.

## 7.4 PI relay proportional gain

Display: ***Ax.P9***  
Range: ***-32.767*** to ***32.767***  
Default Value: ***0.0 10***

Note: the range value may be restricted if the number of display digits does not allow viewing of the full range.

The proportional value will determine the degree to which the controller will respond when there is a difference (error) between the measured value and the process setpoint. If the proportional gain is increased then for a given error the relay on time will be increased (or decreased if the error is on the other side of the setpoint). The proportional gain action can be reversed by setting a negative gain i.e. with a negative gain the on time will reduce as the error increases. With a proportional gain of ***1.000*** and an error of ***10*** or more (with control span set at ***10***) the controller will increase the frequency by 100% if possible. With a proportional gain of ***0.500*** an error of ***10*** or more (with control span set at ***10***) will cause the controller to increase the frequency by 50%, if possible. Too much proportional gain will result in instability due to excessive overshoot of the setpoint. Too little proportional gain will lead to a slow response.

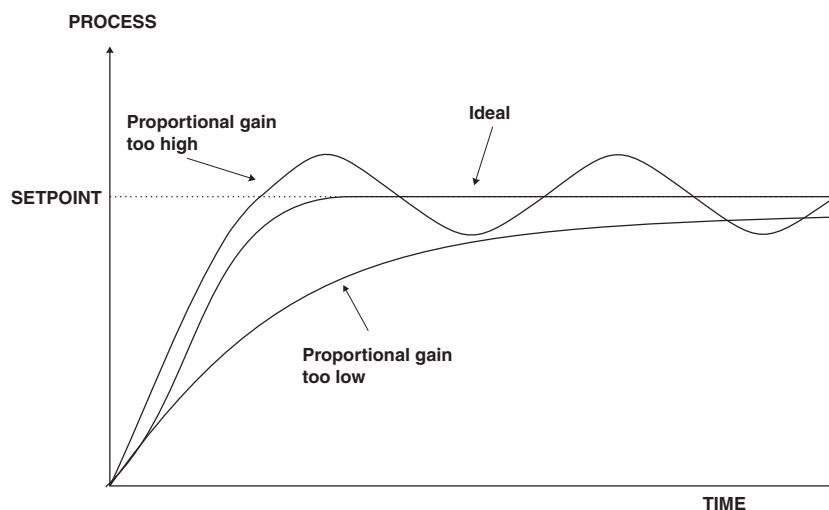

This table shows the effect of the output frequency of changing proportional gain and bias with the following settings: <i>ctrl SPAN = 20, A 1.dc = 1.0, A 1.9 = 0.000</i>			
<b>A 1.SP</b>	<b>A 1.P9</b>	<b>A 1.b5</b>	<b>Effect on relay operation</b>
<b>70</b>	<b>1.000</b>	<b>0.0</b>	Reading of <b>50</b> or below - relay permanently on. Reading of <b>50</b> to <b>70</b> - relay pulses with off time increasing as value approaches <b>70</b> . Reading <b>70</b> or above - relay permanently off.
<b>70</b>	<b>1.000</b>	<b>100.0</b>	Reading of <b>70</b> or below - relay permanently on. Reading of <b>70</b> to <b>90</b> - relay pulses with off time increasing as value approaches <b>90</b> . Reading <b>90</b> or above - relay permanently off.
<b>70</b>	<b>1.000</b>	<b>50.0</b>	Reading of <b>60</b> or below - relay permanently on. Reading of <b>60</b> to <b>70</b> - relay pulses with off time increasing as value approaches <b>70</b> . Reading <b>70</b> - relay pulses at 50% on and 50% off. Reading <b>70</b> to <b>80</b> - relay pulses with off time increasing as value approaches <b>80</b> . Reading <b>80</b> or above - relay permanently off.
<b>70</b>	<b>0.500</b>	<b>50.0</b>	Reading <b>50</b> or below - relay permanently on. Reading <b>50</b> to <b>70</b> - relay pulses with off time increasing as value approaches <b>70</b> . Reading <b>70</b> - relay pulses at 50% on and 50% off. Reading <b>70</b> to <b>90</b> - relay pulses with off time increasing as value approaches <b>90</b> . Reading <b>90</b> or above - relay permanently off.
<b>70</b>	<b>- 1.000</b>	<b>50.0</b>	Reading of <b>60</b> or below - relay permanently off. Reading of <b>60</b> to <b>70</b> - relay pulses with on time increasing as value approaches <b>70</b> . Reading <b>70</b> - relay pulses 50% on and 50% off. Reading <b>70</b> to <b>80</b> - relay pulses with on time increasing as value approaches <b>80</b> . Reading <b>80</b> or above - relay permanently on.

## 7.5 PI relay integral gain

Display: **Ax.1 9**  
 Range: **-32.767** to **32.767**  
 Default Value: **0.000**


Note: the range value may be restricted if the number of display digits does not allow viewing of

the full range.

The Integral action will attempt to correct for any offset which the proportional control action is unable to correct (e.g. errors caused by changes in the process load). When the integral gain is correctly adjusted the control output is varied to maintain control by keeping the process variable at the same value as the control setpoint. Since the integral gain is time based the output will gradually increase if the error does not decrease i.e. if the measured value remains constant and there is an error (a difference between the measured value and the setpoint) then the frequency will be increased compared to the previous frequency output. The higher the proportional gain, the greater the degree by which the on to off ratio will be affected i.e. the response will be greater at higher integral gain settings. With an integral gain of **1.000** an error of **10** or more (with control span set at **10**) will cause the integral action to try to correct at the rate of 100% minute. With an integral gain of **0.200** an error of **10** or more will cause the integral action to try to correct at the rate of 20% per minute. Too high an integral gain will result in instability. Too low an integral gain will slow down the time taken to reach the setpoint. The optimum setting will depend on the lag time of the process and the other control settings. Start with a low figure (e.g. **0.200**) and increase until a satisfactory response time is reached. The integral gain figure has units of gain/minute. The integral action can be reversed by setting a negative gain figure, note that the sign of the integral gain must match the sign of the proportional gain. The integral control output follows the formula:

$$\text{Integral control output} = \frac{\text{error} \times I_g \times \text{time (seconds)}}{60} + \text{previous integral control output}$$

Where  $I_g$  is the integral gain set via **Ax.1 9**.

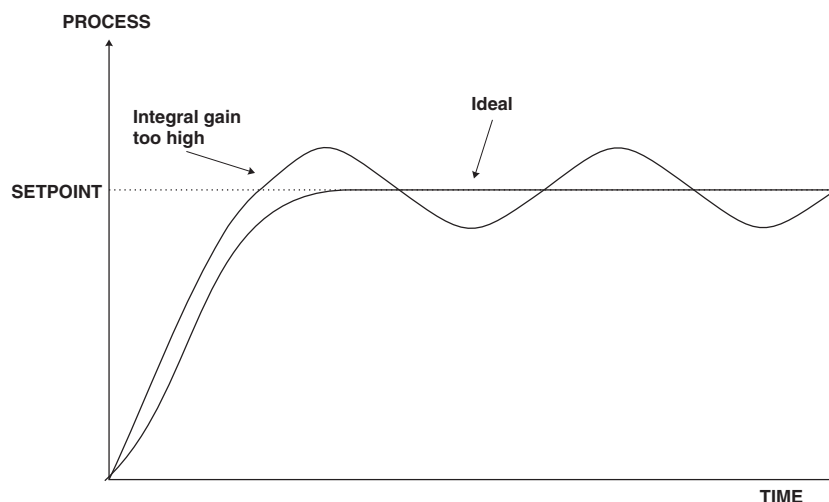

## 7.6 PI relay integral control low limit

**Display:** **Ax.1 L**  
**Range:** **0.0 to 100.0**  
**Default Value:** **100.0**

The minimum limit can be used to reduce overshoot of the control setpoint when the control output is being reduced i.e. falling below the setpoint. The low limit reduces the available output swing by a percentage of the maximum output. Without a limit the integral output can be very large at

the time the setpoint is reached and a large overshoot of the will then result. Settings available are from **0.0** to **100.0** (%). If the limit setting is too high then overshoot will result. If the setting is too low then the integral output can be limited to such an extent that the setpoint cannot be maintained.

Start with a low value such as **20.0** and increase or decrease the value until a satisfactory result is obtained. The advantage of using separate low and high limits is that in many applications the response is very one directional e.g. the system may respond very quickly to a heat input but may cool down at a much slower rate. Separate high and low limit settings allow independent limiting of the integral control swing below and above the setpoint so a smaller minimum limit can be set to limit swings below the setpoint to compensate for the slower cooling time.

The minimum and maximum limits are used in conjunction with the output bias setting to maintain the control process setpoint value. For example with a bias (**Ax.b5**) set at 50%, minimum limit set at 20% and a maximum limit of 30% the actual bias when the process is at the setpoint may be anywhere between 30% and 80% i.e. Integral control is being used to alter the bias setting in order to maintain the process at the setpoint. In this case the minimum term will allow the bias to drop to a value between 50% and 30% in order to maintain the setpoint. The maximum term will allow the bias point to rise to a value between 50% and 80% in order to maintain the setpoint.

## 7.7 PI relay integral control high limit

Display: **Ax.IH**  
Range: **0.0** to **100.0**  
Default Value: **100.0**

The maximum limit can be used to reduce overshoot of the control setpoint when the control output is increasing i.e. rising above the setpoint. Other than this the limit operates in the same manner as the low limit described previously.

## 7.8 PI relay control output bias


Display: **Ax.b5**  
Range: **0.0** to **100.0**  
Default Value: **50.0**

The control bias sets the ideal steady state output required once the setpoint is reached. Settings are in % from **0.0** to **100.0**. When set at **0.0** the relay will be de-activated for the entire control period when the measured input is at the setpoint (depending on proportional and integral gain settings). If set at **50.0** then the relay operation frequency will on for 50% and off for 50% of the duty cycle time when the measured input is at the setpoint. If set at **100.0** then the relay will be activated for the whole time whilst the measured input is at the setpoint.

## 7.9 PI relay control cycle period

**Display:**  $Ax.dc$   
**Range:** 0 to 250  
**Default Value:** 10

Displays and sets the control period cycle from 0 to 250 seconds. The control period sets the total time for each on/off cycle. This time should be set as long as possible to reduce wear of the control relay and the controlling device.

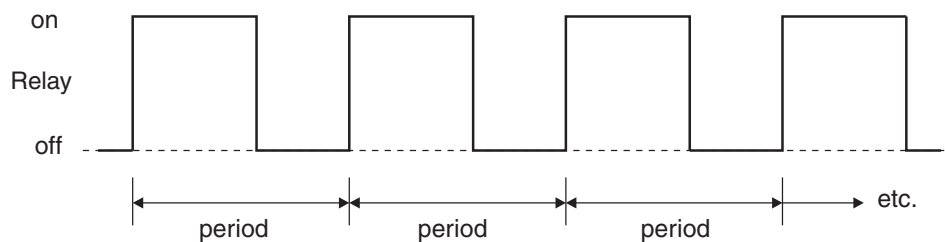

## 7.10 Setting up the PI pulse width controller

1. Set the  $Ax.OPER$  function to  $Ax.tP$ .
2. Set the control setpoint  $Ax.SP$  to the required setting.
3. Set the control span  $ctrl.SPAN$  to the required setting.
4. Set the proportional gain  $Ax.PG$  to an arbitrary value e.g. 0.500.
5. Set the integral gain  $Ax.IG$  to 0.000 (i.e. off).
6. Set the low and high integral  $Ax.I.L$  and  $Ax.I.H$  limits to an arbitrary value e.g. 20.00.
7. Set the bias  $Ax.bS$  to 50.0.
8. Set the cycle  $Ax.dc$  period to 20 seconds.

Initialise the control system and monitor the control results. If the original settings causes process oscillations then gradually decrease the proportional gain until the oscillations decrease to an acceptable steady cycle. If the original settings do not cause process oscillations then gradually increase the proportional gain until a steady process cycling is observed.

Once the steady cycling state is achieved note the difference between the display value and the control setpoint value. Gradually increase or decrease the bias value until the displayed value matches (or cycles about) the control setpoint value.

Gradually increase the integral gain until the process begins to oscillate. Then reduce the integral gain slightly to regain the control without this added oscillation.


Create a step change to the process conditions and observe the control results. It may be necessary to fine tune the settings and use integral limits to obtain optimum results.

Set up sequence	Symptom	Solution
Proportional gain	Slow response	Increase proportional gain
Proportional gain	High overshoot or oscillation	Decrease proportional gain
Proportional bias	Process above or below setpoint	Increase or decrease bias as required
Integral gain	Slow response	Increase integral gain
Integral gain	Instability or oscillations	Decrease integral gain

## 7.11 Relay frequency modulation control mode

To use pulse width modulation control **Rx.Fr** must be selected at the **Rx OPER** function. In frequency modulation mode the relay on time is fixed. A minimum relay off time can also be set. The control program will vary the actual off time to suit the error seen between the setpoint and the measured temperature at the time. For example if extra dosing is needed to reach the setpoint then the off time will be reduced resulting in more on pulses per period of time i.e. the frequency of the pulses is controlled to allow the setpoint to be maintained.

Frequency control - pulse frequency varies according to settings and control requirement

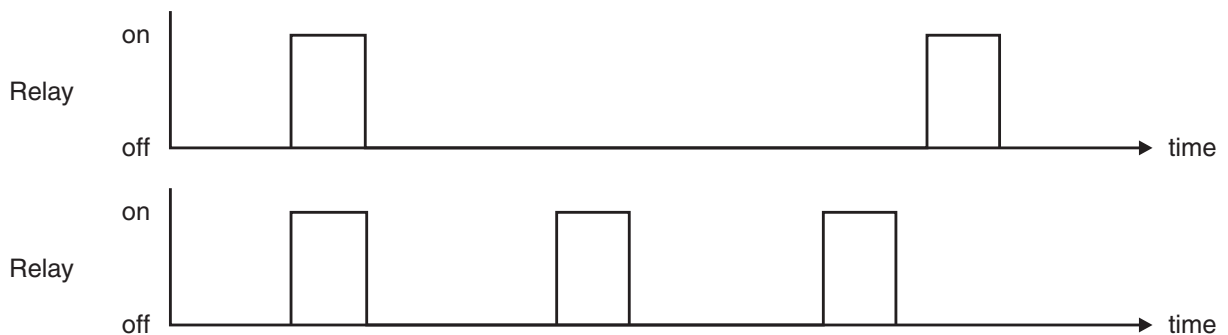

Frequency PI control operation has many functions in common with PI pulse width control, refer to the appropriate sections as shown below for these common functions.

**Rx.SP** (Control setpoint) - refer to section 7.2

**ctrl SPAN** (Control span) - refer to section 7.3

**Rx.PG** (Proportional gain) - refer to section 7.4

**Rx.IG** (Integral gain) - refer to section 7.5

**Rx.LL** (Integral control low limit) - refer to section 7.6

**Rx.HH** (Integral control high limit) - refer to section 7.7

**Rx.bS** (PI control bias) - refer to section 7.8

**Rx.dc** (PI control cycle period) - refer to section 7.9. In frequency mode this function sets the minimum off time. If set to **0** the relay will be disabled. The control program can extend the off time to maintain the setpoint but not reduce it. If a 100% error is seen then the pulse rate will be at its maximum i.e. the off time will equal **Rx.dc**. If a 50% error is seen there will be a pulse every 2 times **Rx.dc**. For a 25% error there will be a pulse every 4 times **Rx.dc** and for a 10% error there will be a pulse every 10 times **Rx.dc**.

This table shows the effect of the output frequency of changing proportional gain and bias with the following settings:  
*ctrl SPAN = 20, A 1.dc = 1.0, A 1.19 = 0.000*

<b>A 1.SP</b>	<b>A 1.P9</b>	<b>A 1.b5</b>	<b>Effect on relay operation</b>
<b>70</b>	<b>1.000</b>	<b>0.0</b>	Reading of <b>50</b> or below - relay pulses at maximum frequency. Reading of <b>50</b> to <b>70</b> - relay pulses with frequency decreasing as value approaches <b>70</b> . Reading <b>70</b> or above - relay permanently off.
<b>70</b>	<b>1.000</b>	<b>100.0</b>	Reading of <b>70</b> or below - relay pulses at maximum frequency. Reading of <b>70</b> to <b>90</b> - relay pulses with frequency decreasing as value approaches <b>90</b> . Reading <b>90</b> or above - relay permanently off.
<b>70</b>	<b>1.000</b>	<b>50.0</b>	Reading of <b>60</b> or below - relay pulses at maximum frequency. Reading of <b>60</b> to <b>80</b> - relay pulses with frequency decreasing as value approaches <b>80</b> . (period increased by 50% at <b>70</b> compared to minimum period e.g. if minimum period is 4 seconds the period at <b>70</b> will be 6 seconds) Reading <b>80</b> or above - relay permanently off.
<b>70</b>	<b>0.500</b>	<b>50.0</b>	Reading <b>50</b> or below - relay pulses at maximum frequency. Reading <b>50</b> to <b>90</b> - relay pulses with frequency decreasing as value approaches <b>90</b> . (period increased by 50% at <b>70</b> compared to minimum period e.g. if minimum period is 4 seconds the period at <b>70</b> will be 6 seconds) Reading <b>90</b> or above - relay permanently off.
<b>70</b>	<b>- 1.000</b>	<b>50.0</b>	Reading of <b>60</b> or below - relay permanently off. Reading of <b>60</b> to <b>80</b> - relay pulses with frequency decreasing as value approaches <b>80</b> . (period increased by 50% at <b>70</b> compared to minimum period e.g. if minimum period is 4 seconds the period at <b>70</b> will be 6 seconds) Reading <b>80</b> or above - relay pulses at maximum frequency.

## 7.12 PI relay on duration

Display: **Ax.dr**  
Range: **0.0 to 25.0**  
Default Value: **1.0**

Displays and sets the control relay on duration from **0.0** to **25.0** seconds. If set to **0.0** the relay will be disabled. The duration should be long enough to ensure that the device being controlled receives an acceptable on pulse.

### 7.13 Setting up the PI frequency controller

1. Set the ***Ax OPEr*** function to ***AxFr***.
2. Set the control setpoint ***Ax.SP*** to the required setting.
3. Set the control span ***ctrl SPAN*** to the required setting.
4. Set the proportional gain ***Ax.P9*** to an arbitrary value e.g. ***0.500***.
5. Set the integral gain ***Ax.I 9*** to ***0.000*** (i.e. off).
6. Set the low and high integral ***Ax.I L*** and ***Ax.I H*** limits to an arbitrary value e.g. ***20.00***.
7. Set the bias ***Ax.bs*** to ***50.0***.
8. Set the cycle ***Ax.dc*** period to ***20*** seconds.
9. Set the relay on time ***Ax.dr*** to an arbitrary value e.g. ***1.0***

Initialise the control system and monitor the control results. If the original settings causes process oscillations then gradually decrease the proportional gain until the oscillations decrease to an acceptable steady cycle. If the original settings do not cause process oscillations then gradually increase the proportional gain until a steady process cycling is observed.

Once the steady cycling state is achieved note the difference between the display value and the control setpoint value. Gradually increase or decrease the bias value until the displayed value matches (or cycles about) the control setpoint value.

Gradually increase the integral gain until the process begins to oscillate. Then reduce the integral gain slightly to regain the control without this added oscillation.

Create a step change to the process conditions and observe the control results. It may be necessary to fine tune the settings and use integral limits to obtain optimum results.

<b>Set up sequence</b>	<b>Symptom</b>	<b>Solution</b>
Proportional gain	Slow response	Increase proportional gain
Proportional gain	High overshoot or oscillation	Decrease proportional gain
Proportional bias	Process above or below setpoint	Increase or decrease bias as required
Integral gain	Slow response	Increase integral gain
Integral gain	Instability or oscillations	Decrease integral gain

## 8 Specifications

### 8.1 Technical specifications

Input type:	Link selectable $\pm 2\text{mA}$ , $\pm 20\text{mA}$ , 4 to 20mA or DC Volts $\pm 100\text{mV}$ , $\pm 1\text{V}$ , $\pm 10\text{V}$ , $\pm 100\text{V}$ or Slidewire, 3 wire 0-1k $\Omega$ to 0-1M $\Omega$ value slidewires
Impedance:	Typically 150 $\Omega$ for mA input (82 $\Omega$ plus polyfuse resistance) 1M $\Omega$ on DC voltage input
ADC Resolution:	1 in 20,000
Accuracy:	0.1% of input range selected when calibrated (0.3% on $\pm 100\text{mV}$ and $\pm 2\text{mA}$ ranges)
Sample Rate:	4 samples per second
Display update:	4 times per second
Conversion Method:	Dual Slope ADC
Microprocessor:	HC68HC11F CMOS
Ambient temperature:	LED -10 to 60° C, LCD -10 to 50° C
Humidity:	5 to 95% non condensing
Display:	LED Models: 4 digit 20mm, 5 digit 14.2mm + status LEDs + 4 way keypad. 6 digit 14.2mm + 4 way keypad LED Bar Graph 20 segment bar + 5 digit 7.6mm + relay status LEDs LED Circular Bar Graph 16 segment + 5 digit 7.6mm + relay status LEDs LCD Models: 4 digit 12.7mm, 6 digit 12.7mm
Power Supply:	AC 240V, 110V or 24V 50/60Hz or DC isolated wide range 12 to 48V. Special supply types 32VAC, 48VAC 50/60Hz or DC isolated 50 to 110V also available. Note: supply type is factory configured.
Power Consumption:	AC supply 4 VA max, DC supply typically 160mA at 12VDC and 80mA at 24VDC for PM4 with no optional outputs, actual current drawn depends on display type and options fitted
Output (standard):	1 x relay, Form A, rated 5A resistive 18VDC (approx.) non isolated regulated transmitter supply (25mA max.)
Relay Action:	Programmable N.O. or N.C or PI control (frequency or pulse width)

### 8.2 Optional outputs

Extra Relays:	Same specs. as Relay 1 (up to 6 extra relays). The standard relay and first optional relay can be programmed for PI control operation if required. Available as one, three or six extra relays.
Analog Retransmission:	12 bit isolated 4 to 20mA, 0 to 1V or 0 to 10V link selectable (single or dual analog output versions available). (4-20mA will drive into resistive loads of up to 800 $\Omega$ )
Digital Retransmission:	Isolated BCD/Binary
Serial Communications:	Isolated RS232 or RS485 (ASCII or Modbus RTU)
DC Voltage Output:	Isolated $\pm 12\text{V}(24\text{V})$ standard, $\pm 5\text{V}(10\text{V})$ link selectable (rated at 25mA).

### 8.3 Physical Characteristics

Bezel Size:	DIN 48mm x 96mm x 10mm
Case Size:	44mm x 91mm x 120mm behind face of panel
Panel Cut Out:	45mm x 92mm +1mm/-0mm
Connections:	Plug in screw terminals (max. 2.5mm <sup>2</sup> wire)
Weight:	400 gms basic model, 450 gms with option card

## 9 Guarantee and service

The product supplied with this manual is guaranteed against faulty workmanship for a period of two years from the date of dispatch.

Our obligation assumed under this guarantee is limited to the replacement of parts which, by our examination, are proved to be defective and have not been misused, carelessly handled, defaced or damaged due to incorrect installation. This guarantee is VOID where the unit has been opened, tampered with or if repairs have been made or attempted by anyone except an authorised representative of the manufacturing company.

Products for attention under guarantee (unless otherwise agreed) must be returned to the manufacturer freight paid and, if accepted for free repair, will be returned to the customers address in Australia free of charge.

When returning the product for service or repair a full description of the fault and the mode of operation used when the product failed must be given. In any event the manufacturer has no other obligation or liability beyond replacement or repair of this product.

Modifications may be made to any existing or future models of the unit as it may deem necessary without incurring any obligation to incorporate such modifications in units previously sold or to which this guarantee may relate.

This document is the property of the instrument manufacturer and may not be reproduced in whole or part without the written consent of the manufacturer.

This product is designed and manufactured in Australia.